Calibration transfers a HuSkin−trained model to independent SkinPiX measurements

HuSkinDB was used for model fitting only; evaluation used 54 SkinPiX−only compounds from four unseen sources

A

One shared compound calibrates a completely unseen source

Open circle = HuSkin prediction; filled circle = after one−anchor source calibration

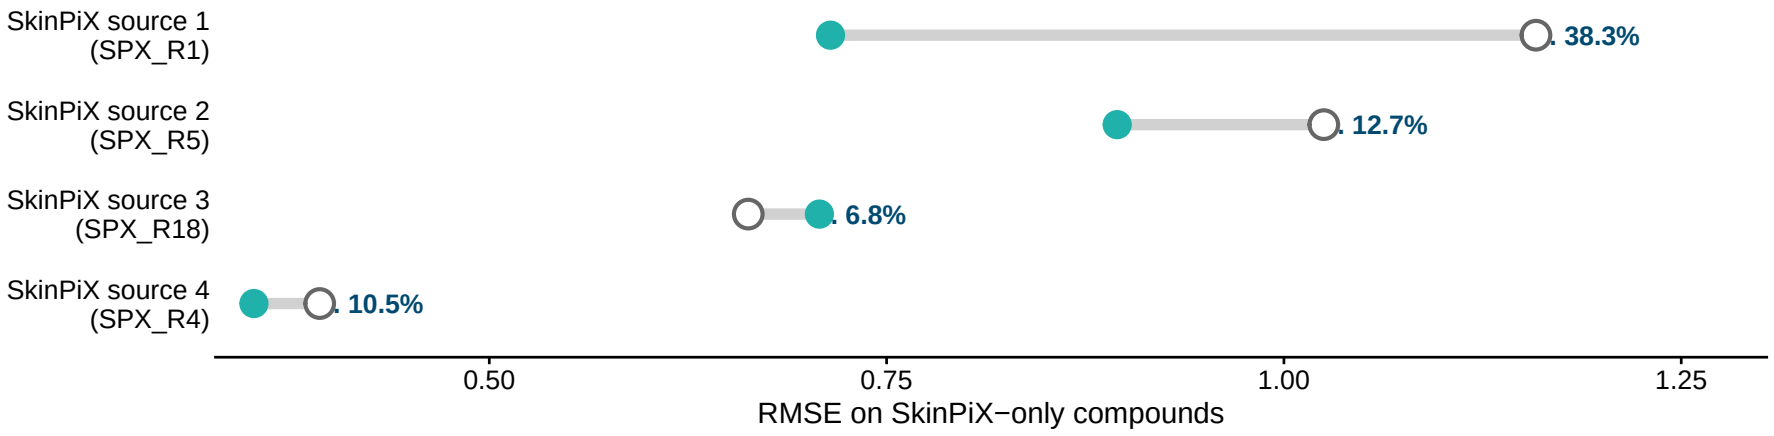

B

Calibration reduces error for most external compounds

44/54 SkinPiX−only compounds move below the identity line

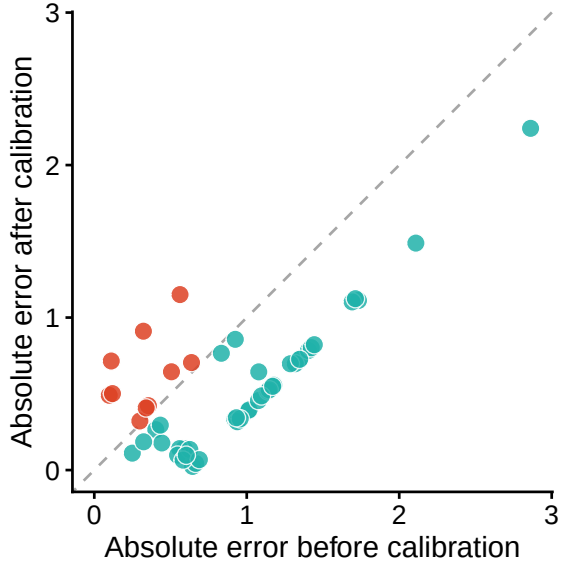

C

More shared compounds provide additional calibration informati

Colored lines are the same three external sources; dark blue is their aggregate RM

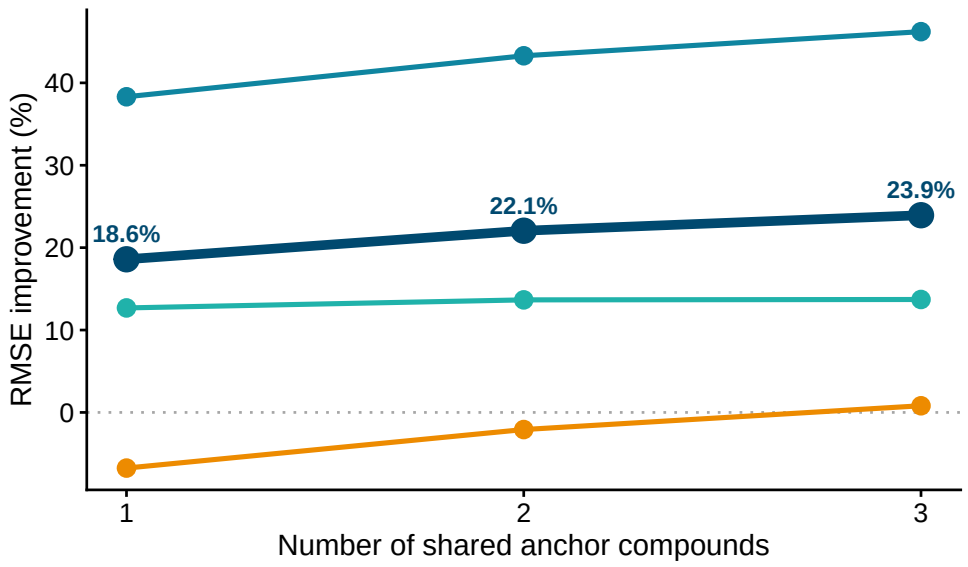

Higher error after calibration Lower error after calibration

SPX_R1 SPX_R18 SPX_R5