Calibration transfers a HuSkin−trained model to SkinPiX measurements

Evaluation used SkinPiX−only compounds from four sources not used for HuSkin model fitting

A

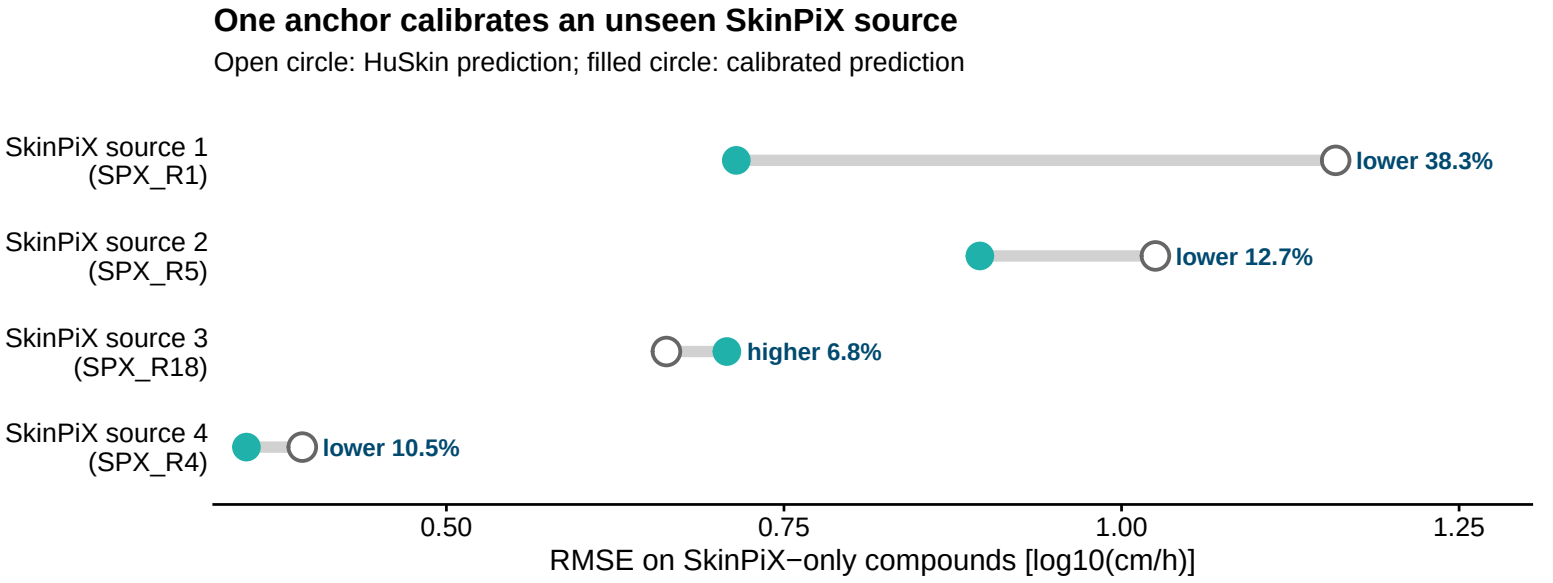

B

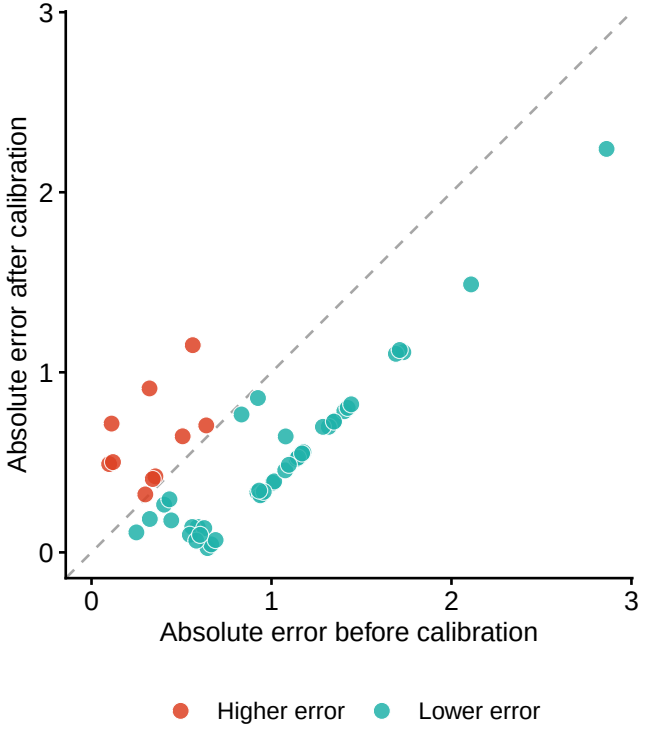
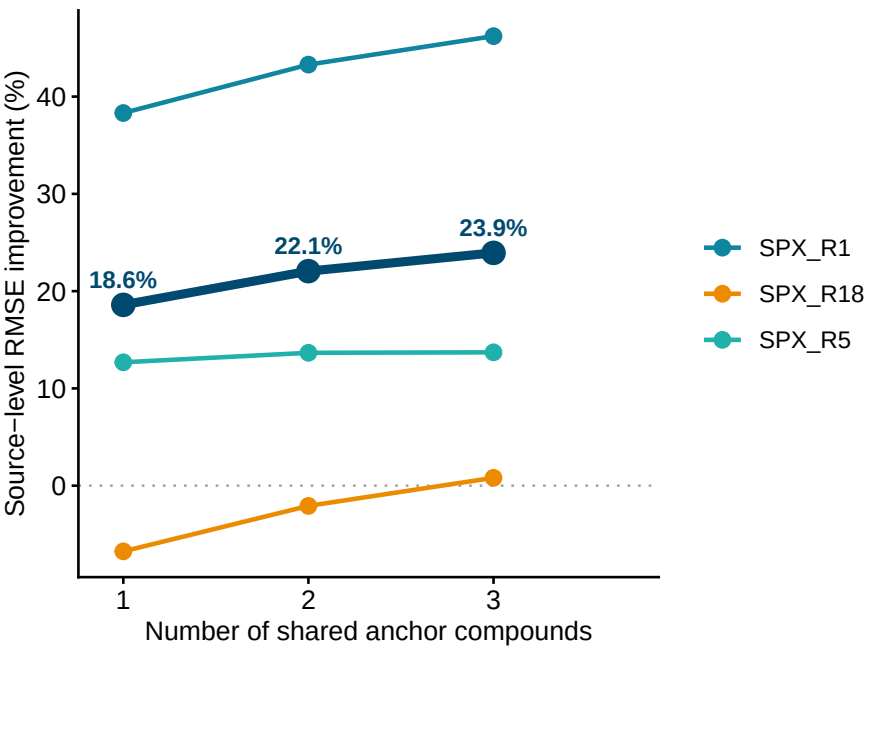
C