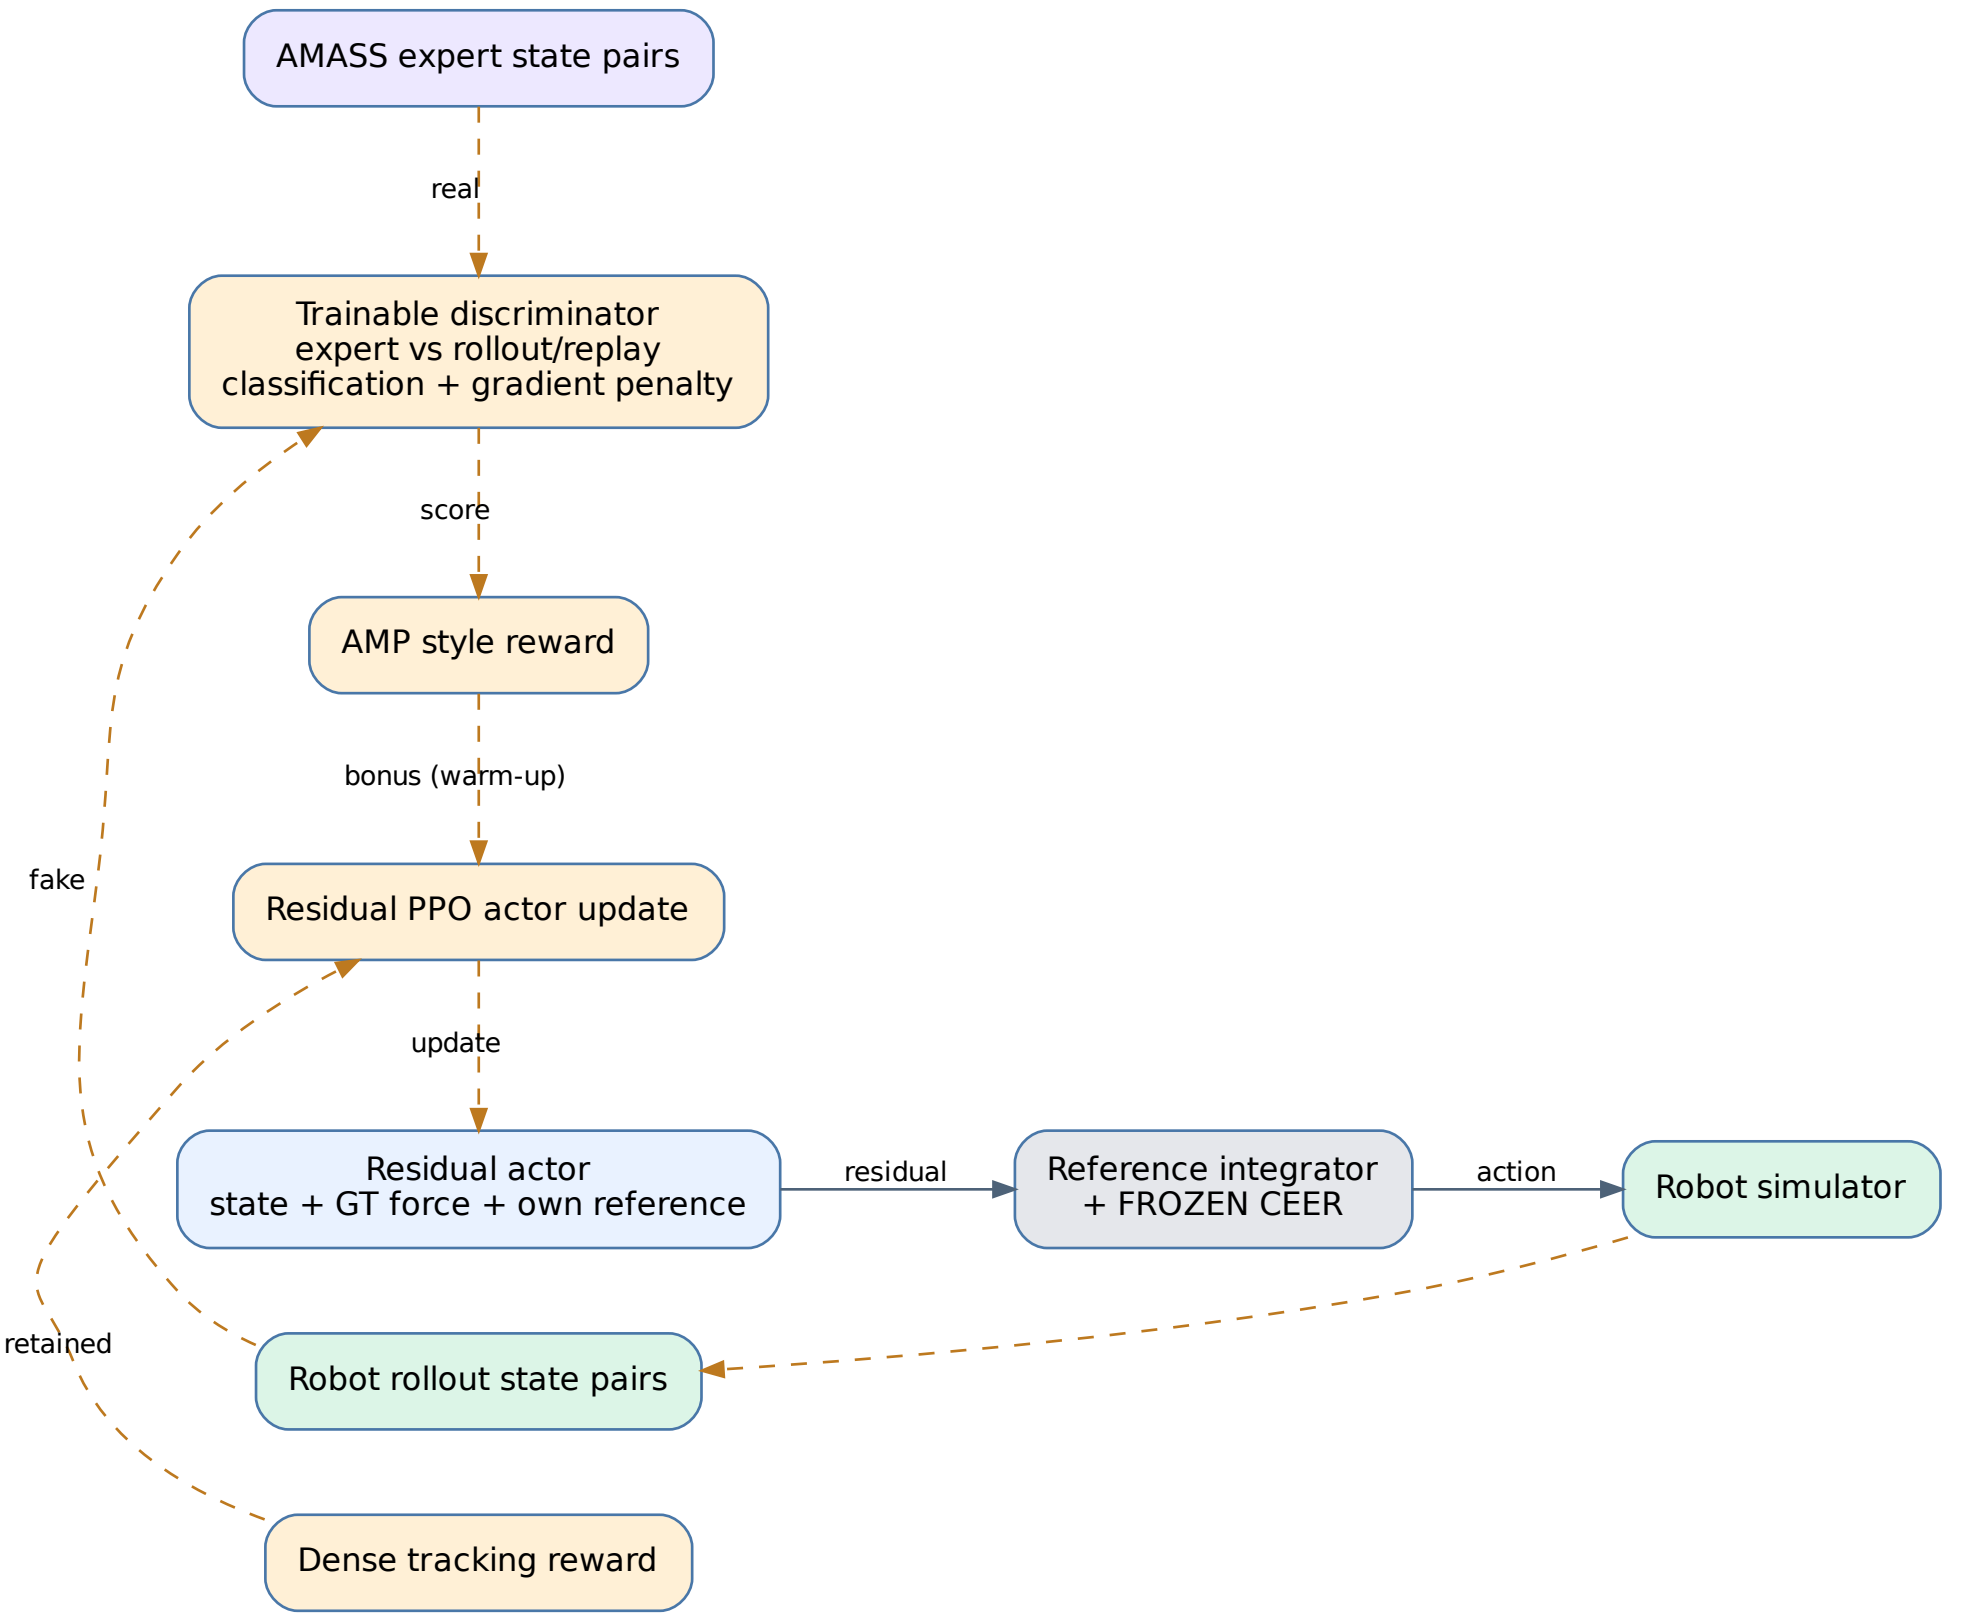D | Dense tracking + AMP motion-prior ablation