




Certificate of Hydrophone Calibration

Hydrophone:	Onda HGL-0400 S/N: 1037
Cable/Adaptor:	NONE
External Amplifier:	NONE
Electrical Loading:	OpenCircuit
Temperature:	23.5 deg C
Calibration Completed:	10-Jun-2024
Data File Name:	HGL0400-1037_XXXXXX-XXXX-XX_XX_20240610.txt

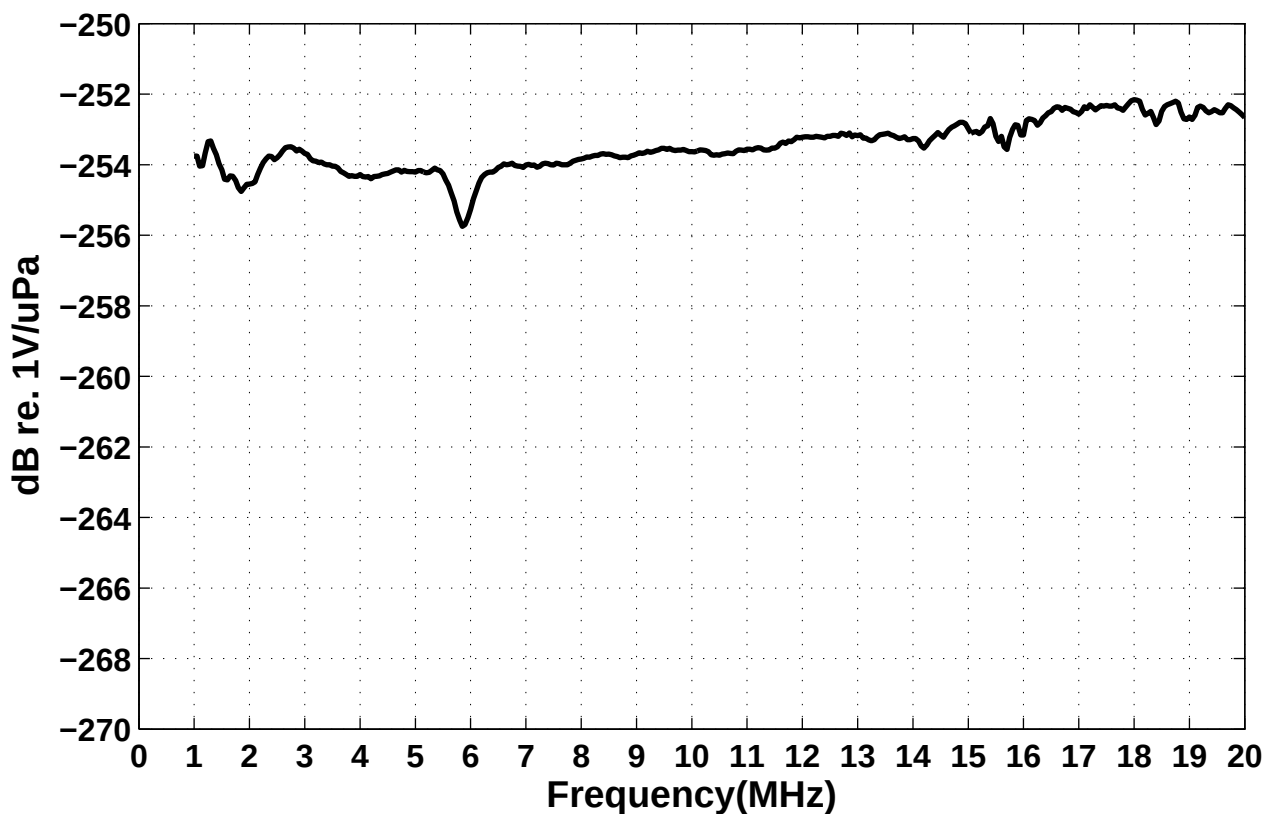

Calibration Method: Stepped single frequency comparison to Reference Standard

Measurement Uncertainty: 1-15 MHz: 1 dB; 15-20 MHz: 1.5 dB

Signature: *Samuel M. Howard* Date: 10-Jun-2024

1290 Hammerwood Avenue, Sunnyvale, CA 94089 T: (408) 745-0383 F: (408) 745-0956
www.ondacorp.com