


IS Voyager Mobile System Installation Guide

Step 3-5


For IS 3800W

Power adapter connects to handpiece charging station with the wire going through the handle

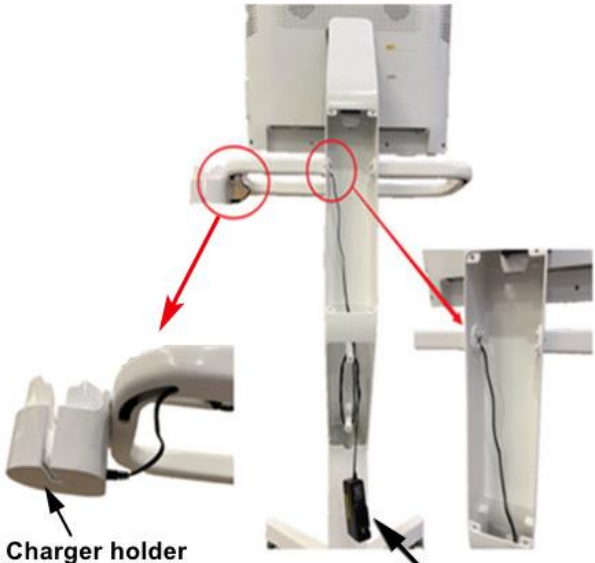

For IS 3600 / IS 3700

Power adapter connects to power box with the wire going through the front hole on the display stem

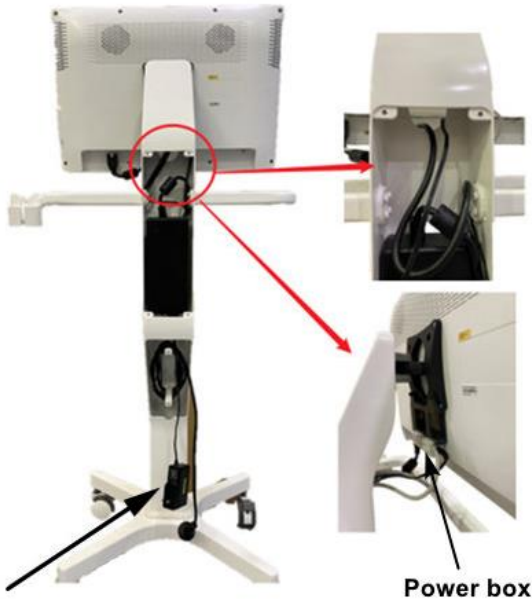

⑥ Power adapter of intraoral scanner




IMPORTANT: This step can be skipped for IS 3800 which doesn't supply a power adapter.

Step 3-6

Reattach rear cover and lower cover to the display stem referring to **Step 3-4**.

Step 3-7

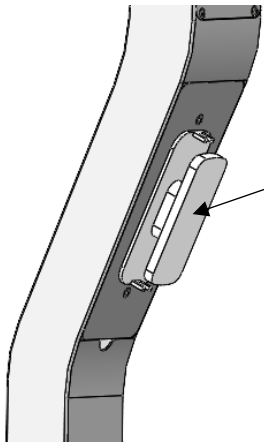


Power strip hook for extension cable storage



IMPORTANT: Two pieces of double-sided tape are available along with the power strip hook.

1. System and Component Overview

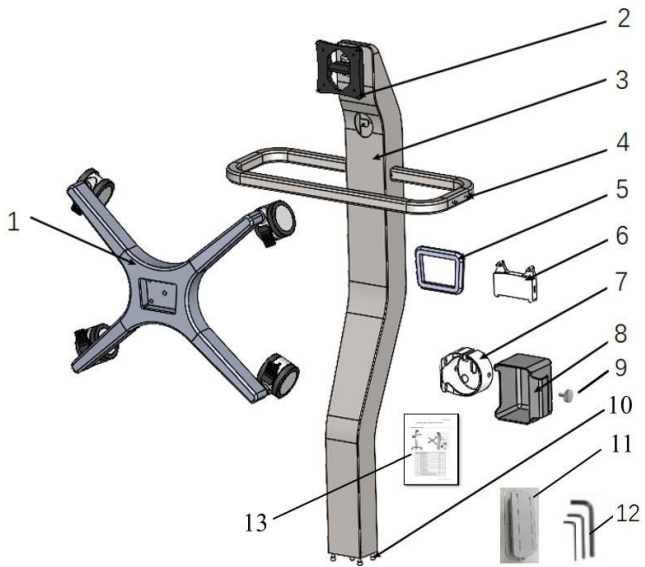

Index	Description	Qty.
1	Wheel base	1
2	Screw M4x12	4
3	Display stem	1
4	Screw M4x20	4
5	Rubber ring	1
6	Adapter base	1
7	Charger holder	1
8	Basket	1
9	Plastic knurled screw M4x10	4
10	Screw M6x20	4
11	Power strip hook	1
12	Installation tool (Allen wrench)	3
13	Installation guide (this document)	1

Note: The usage and maintenance of the AIO Medical PC and the intraoral scanner are not covered by this guide.



WARNINGS




- Keep all wheels unlocked and in contact with the floor when moving IS Voyager.
- Do NOT mount any other all-in-one PC not provided by Dental Imaging Technologies Corporation on IS Voyager.
- Always place the scanner in its intended mount on IS Voyager when not in use and when moving IS Voyager.
- Do NOT place IS Voyager on a slope greater than 10 degrees.

Cleaning and disinfecting: During normal use, IS Voyager may become dirty and should be cleaned regularly. Prepare a clean cloth that has been moistened in a cleaning solution, and wipe IS Voyager thoroughly with the cloth. Or use cleaning wipes.

Tested cleaning agents: 75% Alcohol, CaviWipes




2. Display Stem Installation

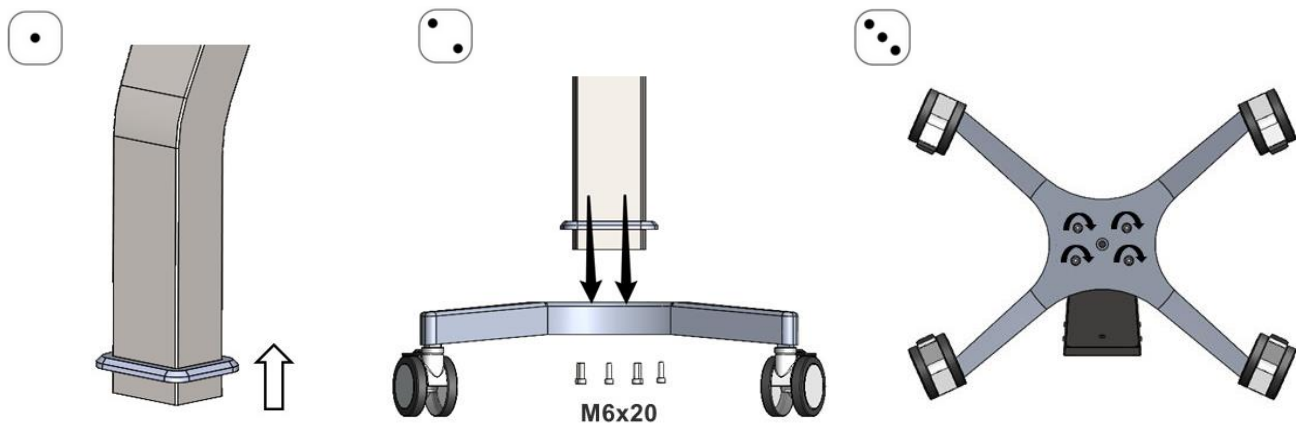


3. Accessory Installation


Step 3-1

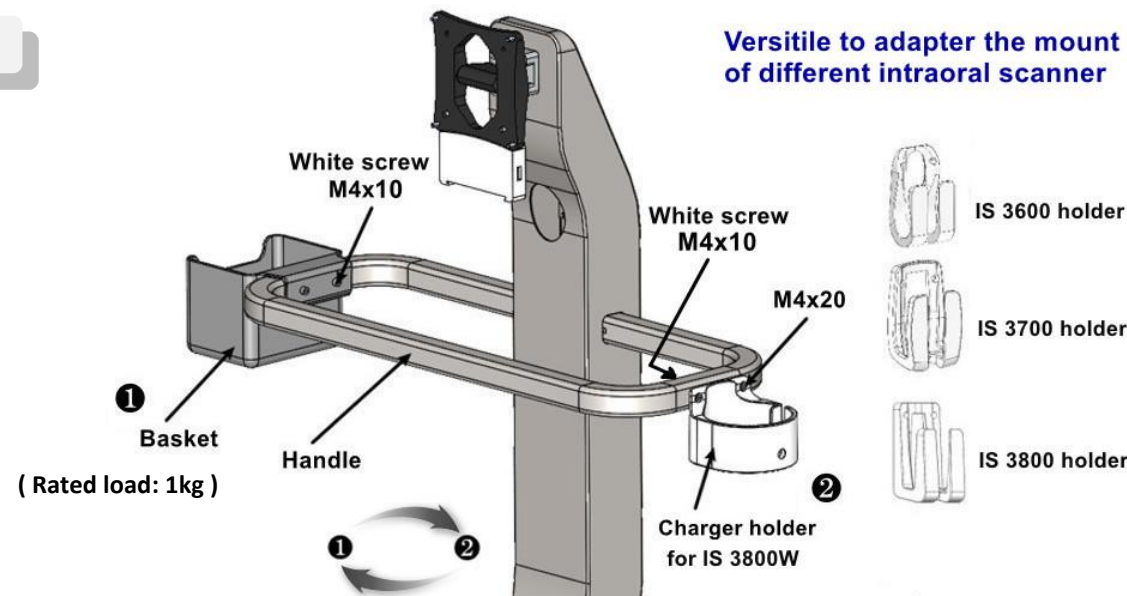


Step 3-2

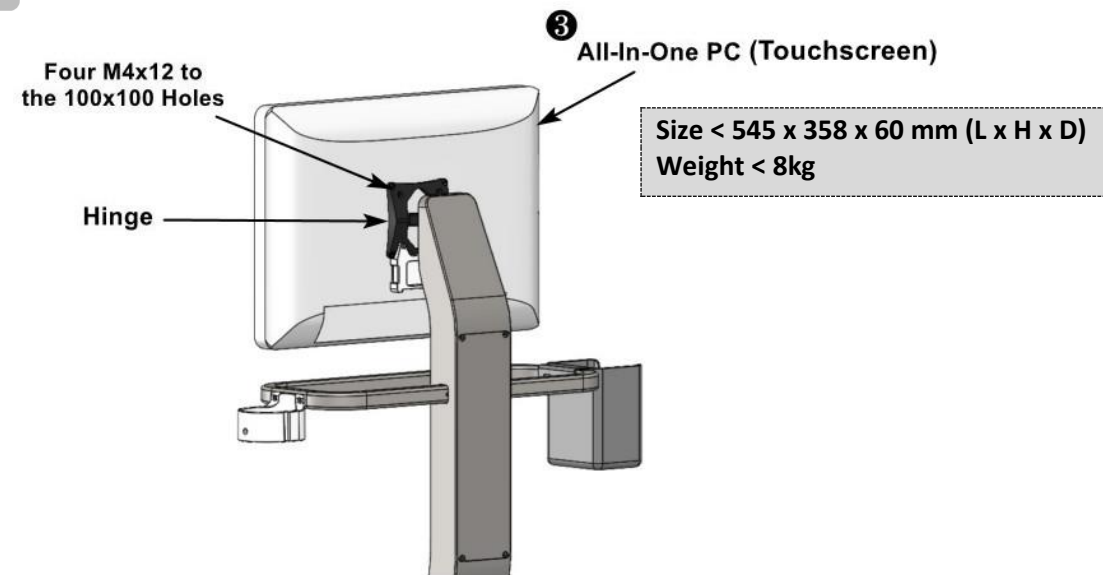


Step 3-3

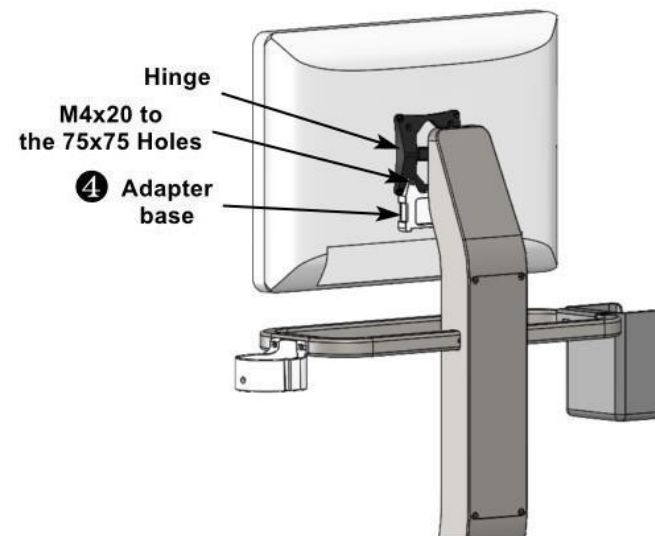

For IS 3600 / IS 3700

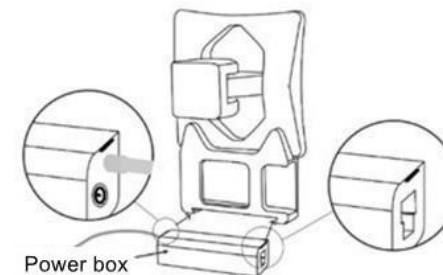

For IS 3800W

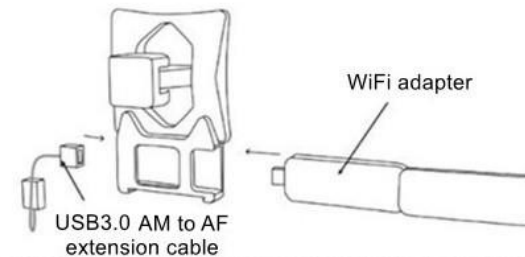

For IS 3800

Adapter base is not used.
Direct connection to PC with a USB2.0 AM to Type-C F converter.



IMPORTANT: The USB3.0 extension cable and the USB2.0 to USB-C converter are available along with the customized all-in-one medical PC.

Step 3-4

