



Detiding Validation: 30-Day Calibration Data


(a) Full-fit residual RMS

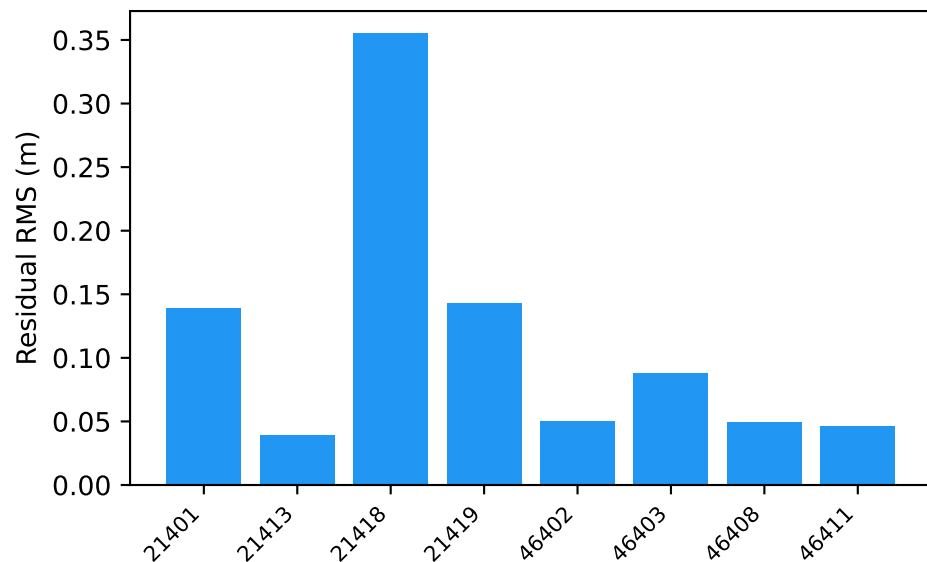

(b) Holdout validation RMS

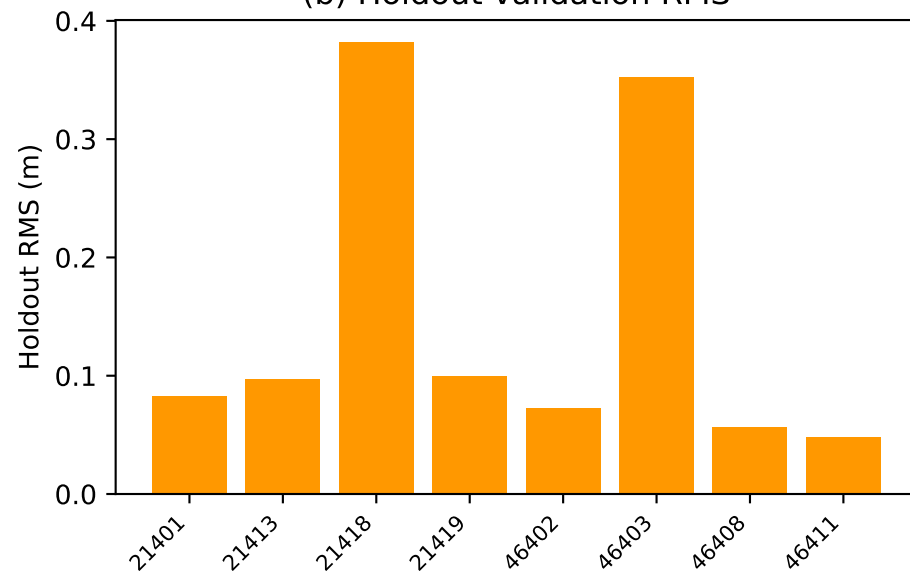

(c) M2 constituent amplitude

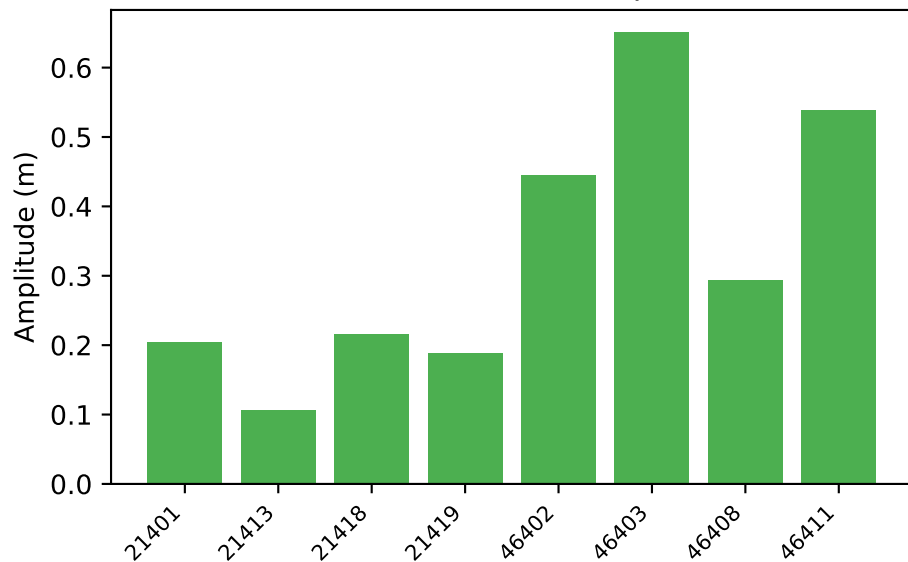

(d) S2 constituent amplitude

