


Beat 1 of 5 | Segment 1780110624672_VC2B008BF_184B27_ecg_seg0

Beat index 2 | t = 2.832 s | Pipeline confidence: 100.0%

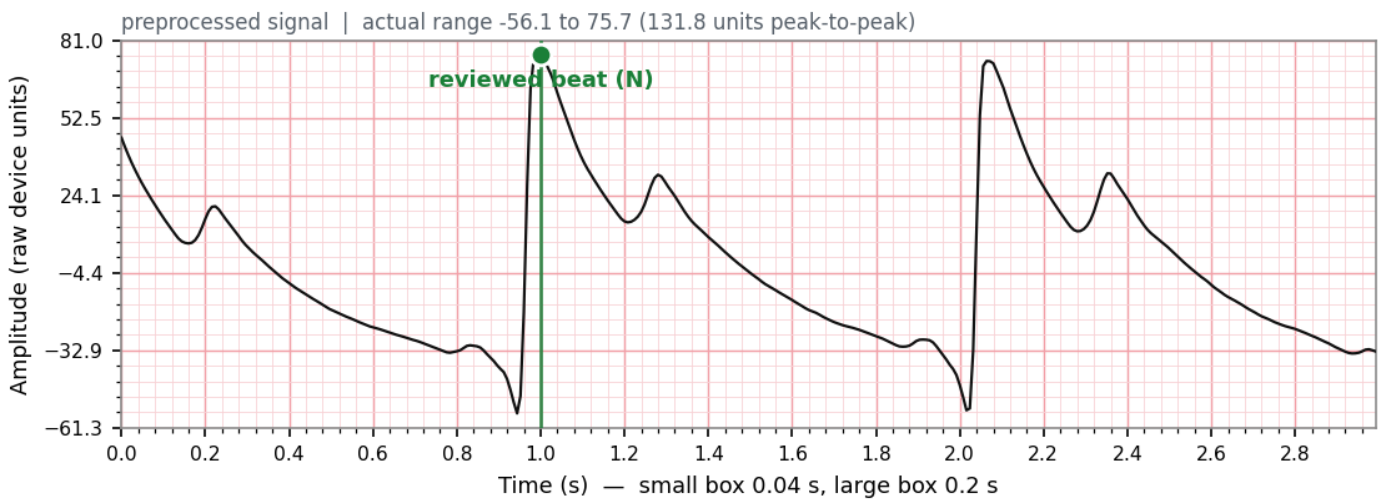

Pipeline predicted: N (Normal sinus beat) — Confidence: 100.0%

Rhythm context: N → [N] → N

RR before: 1080 ms RR after: 1064 ms

Q1. What is your label for this beat?

- ☐ N — Normal sinus beat
- ☐ S — Supraventricular (PAC, junctional)
- ☐ V — Ventricular (PVC, ectopic)
- ☐ F — Fusion beat
- ☐ Q — Artifact / uninterpretable
- ☐ Unsure — needs more context

Q2. Signal quality for this beat?

- ☐ Clean — usable for analysis
- ☐ Noisy — interpret with caution
- ☐ Artifact — discard this beat

Q3. Do you agree with the pipeline prediction?

- ☐ Yes — pipeline is correct
- ☐ No — pipeline is wrong (my label above is correct)
- ☐ Borderline — could be either

Q4. If you answered V or S above — clinically significant?


(skip if not applicable)

- ☐ Isolated — not concerning
- ☐ Part of a run — concerning
- ☐ Unsure

Comment (optional):

Beat 2 of 5 | Segment 1780110624672_VC2B008BF_184B27_ecg_seg0

Beat index 5 | t = 6.056 s | Pipeline confidence: 100.0%

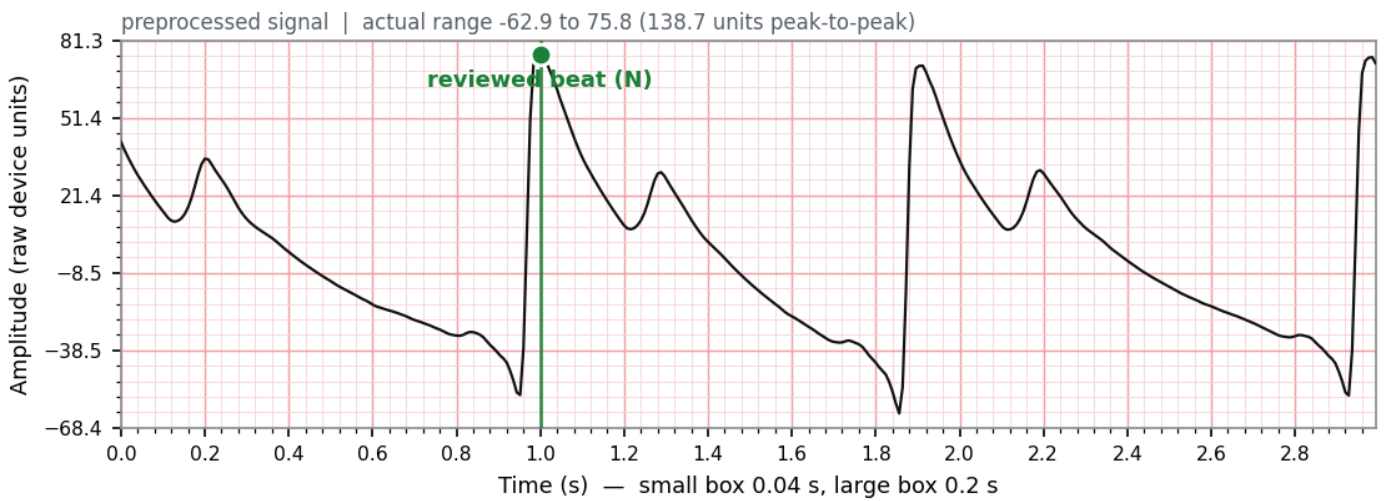

Pipeline predicted: N (Normal sinus beat) — Confidence: 100.0%

Rhythm context: N → [N] → N

RR before: 1080 ms RR after: 912 ms

Coupling interval 912 ms is 16% shorter than the preceding RR — early beat.

Q1. What is your label for this beat?

- ☐ N — Normal sinus beat
- ☐ S — Supraventricular (PAC, junctional)
- ☐ V — Ventricular (PVC, ectopic)
- ☐ F — Fusion beat
- ☐ Q — Artifact / uninterpretable
- ☐ Unsure — needs more context

Q2. Signal quality for this beat?

- ☐ Clean — usable for analysis
- ☐ Noisy — interpret with caution
- ☐ Artifact — discard this beat

Q3. Do you agree with the pipeline prediction?

- ☐ Yes — pipeline is correct
- ☐ No — pipeline is wrong (my label above is correct)
- ☐ Borderline — could be either

Q4. If you answered V or S above — clinically significant?


(skip if not applicable)

- ☐ Isolated — not concerning
- ☐ Part of a run — concerning
- ☐ Unsure

Comment (optional):

Beat 3 of 5 | Segment 1780110624672_VC2B008BF_184B27_ecg_seg0

Beat index 12 | t = 11.8 s | Pipeline confidence: 91.0%

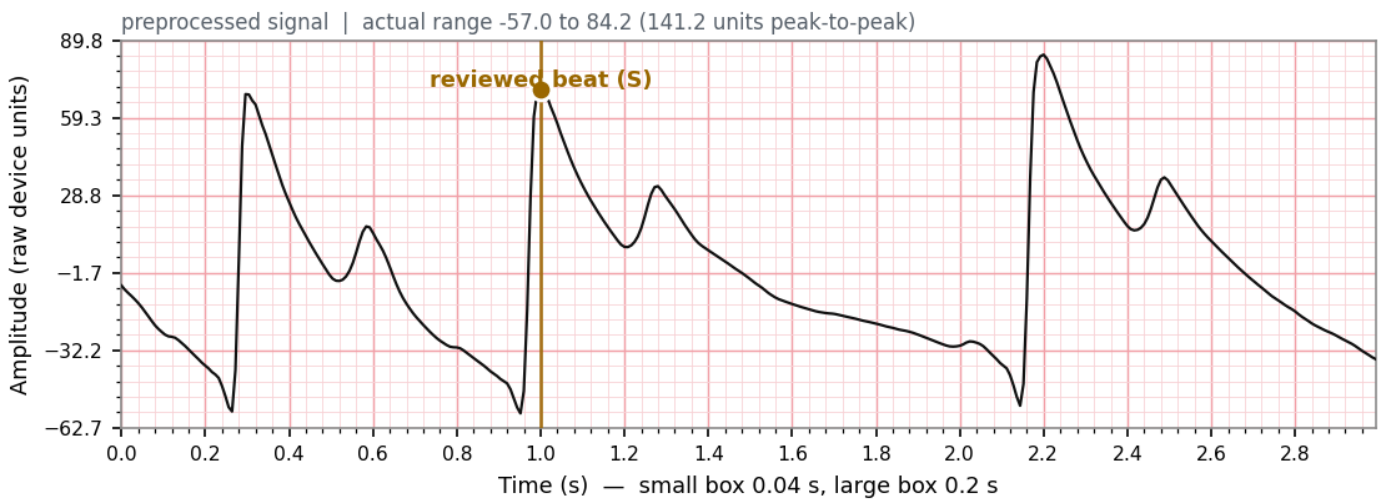

Pipeline predicted: S (Supraventricular (PAC, junctional)) — Confidence: 91.0%

Rhythm context: N → [S] → N

RR before: 704 ms RR after: 1200 ms

Following interval 1200 ms exceeds the preceding RR — possible pause (interval is fully measured).

Q1. What is your label for this beat?

- ☐ N — Normal sinus beat
- ☐ S — Supraventricular (PAC, junctional)
- ☐ V — Ventricular (PVC, ectopic)
- ☐ F — Fusion beat
- ☐ Q — Artifact / uninterpretable
- ☐ Unsure — needs more context

Q2. Signal quality for this beat?

- ☐ Clean — usable for analysis
- ☐ Noisy — interpret with caution
- ☐ Artifact — discard this beat

Q3. Do you agree with the pipeline prediction?

- ☐ Yes — pipeline is correct
- ☐ No — pipeline is wrong (my label above is correct)
- ☐ Borderline — could be either

Q4. If you answered V or S above — clinically significant?


(skip if not applicable)

- ☐ Isolated — not concerning
- ☐ Part of a run — concerning
- ☐ Unsure

Comment (optional):

Beat 4 of 5 | Segment 1780110624672_VC2B008BF_184B27_ecg_seg0

Beat index 15 | t = 14.736 s | Pipeline confidence: 55.7%

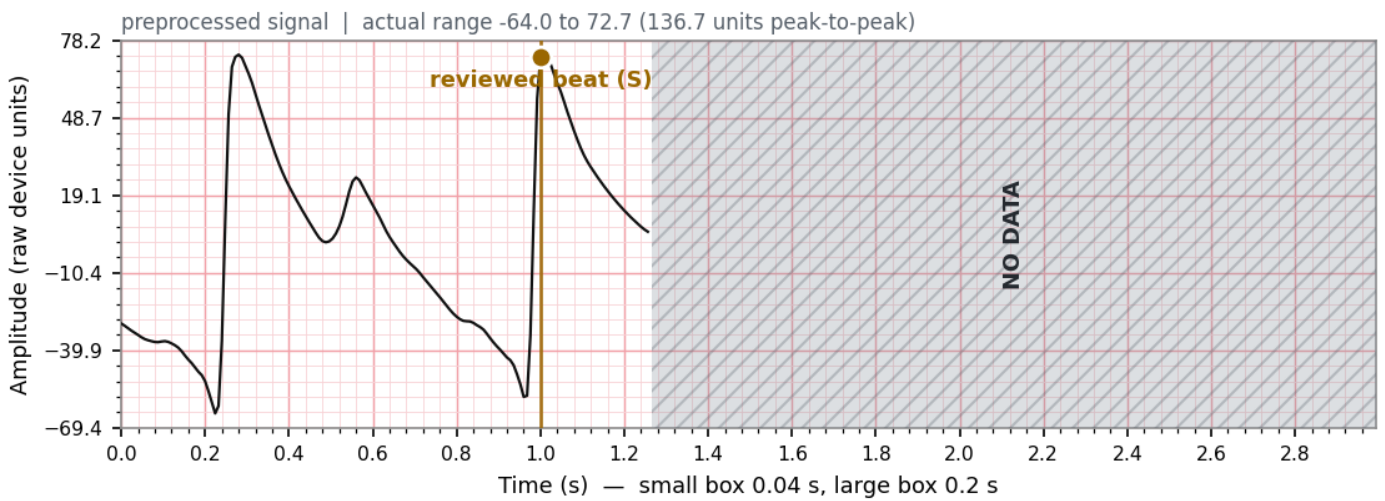

Pipeline predicted: S (Supraventricular (PAC, junctional)) — Confidence: 55.7%

Rhythm context: N → [S] → N

RR before: 720 ms RR after: 5504 ms

RR-after (5504 ms) spans removed data — NOT a measured pause. Do not interpret as asystole.

58% of this 3 s strip is removed data (shaded NO DATA) — not recorded signal.

Q1. What is your label for this beat?

- ☐ N — Normal sinus beat
- ☐ S — Supraventricular (PAC, junctional)
- ☐ V — Ventricular (PVC, ectopic)
- ☐ F — Fusion beat
- ☐ Q — Artifact / uninterpretable
- ☐ Unsure — needs more context

Q2. Signal quality for this beat?

- ☐ Clean — usable for analysis
- ☐ Noisy — interpret with caution
- ☐ Artifact — discard this beat

Q3. Do you agree with the pipeline prediction?

- ☐ Yes — pipeline is correct
- ☐ No — pipeline is wrong (my label above is correct)
- ☐ Borderline — could be either

Q4. If you answered V or S above — clinically significant?

(skip if not applicable)


- ☐ Isolated — not concerning
- ☐ Part of a run — concerning
- ☐ Unsure

Comment (optional):

This is a pseudo-label review, not a diagnosis.

Beat 5 of 5 | Segment 1780110624672_VC2B008BF_184B27_ecg_seg0

Beat index 43 | t = 44.592 s | Pipeline confidence: n/a (deterministic quality gate, not a model score)

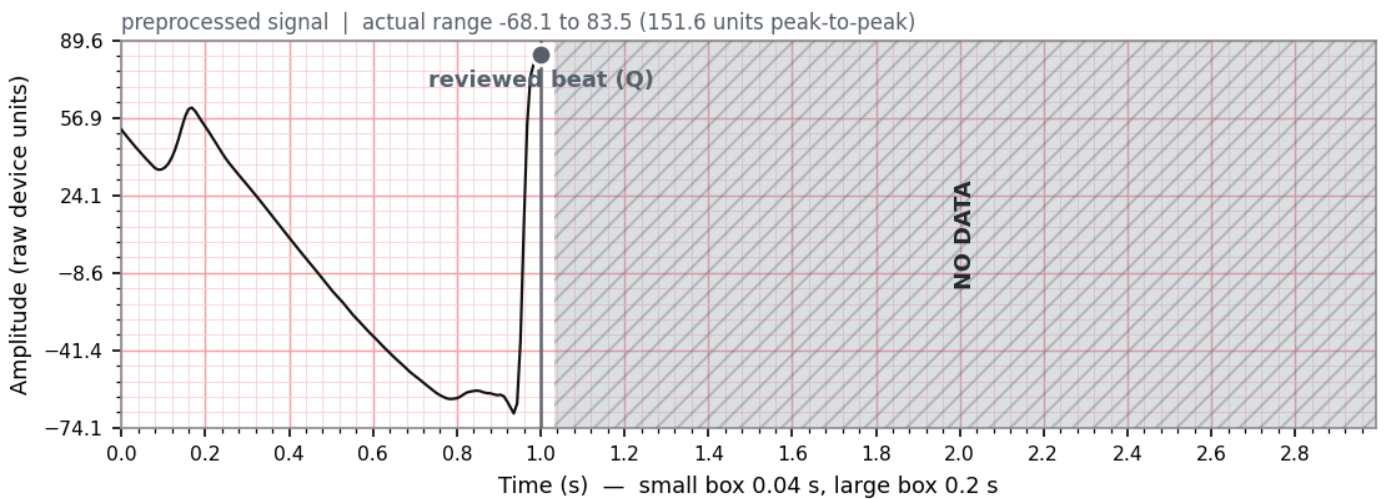

Pipeline predicted: Q (Artifact / uninterpretable) — Confidence: n/a (deterministic quality gate, not a model score)

Rhythm context: N → [Q] → —

RR before: 1120 ms RR after: n/a

66% of this 3 s strip is removed data (shaded NO DATA) — not recorded signal.

Flagged by quality gate: WINDOW_OUT_OF_BOUNDS

Q1. What is your label for this beat?

- ☐ N — Normal sinus beat
- ☐ S — Supraventricular (PAC, junctional)
- ☐ V — Ventricular (PVC, ectopic)
- ☐ F — Fusion beat
- ☐ Q — Artifact / uninterpretable
- ☐ Unsure — needs more context

Q2. Signal quality for this beat?

- ☐ Clean — usable for analysis
- ☐ Noisy — interpret with caution
- ☐ Artifact — discard this beat

Q3. Do you agree with the pipeline prediction?

- ☐ Yes — pipeline is correct
- ☐ No — pipeline is wrong (my label above is correct)
- ☐ Borderline — could be either

Q4. If you answered V or S above — clinically significant?

(skip if not applicable)

- ☐ Isolated — not concerning
- ☐ Part of a run — concerning
- ☐ Unsure

Comment (optional):

This is a pseudo-label review, not a diagnosis.

Pipeline version: ecg_inference/five_class_xgb.json | Page 5/5
Segment: 1780110624672_VC2B008BF_184B27_ecg_seg0 | Amplitude: raw device units (uncalibrated, not mV)
Signal shown: preprocessed (baseline-removed, notch, bandpass, Kalman EMG)

Review summary

5 beat(s) in this document. Answers are stored in the form fields on each page.

Page	Beat idx	Segment	Predicted	Conf.	Context
1	2	1780110624672_VC2B008BF_184B27_ecg_seg0	N	100.0%	N→[N]→N
2	5	1780110624672_VC2B008BF_184B27_ecg_seg0	N	100.0%	N→[N]→N
3	12	1780110624672_VC2B008BF_184B27_ecg_seg0	S	91.0%	N→[S]→N
4	15	1780110624672_VC2B008BF_184B27_ecg_seg0	S	55.7%	N→[S]→N
5	43	1780110624672_VC2B008BF_184B27_ecg_seg0	Q	n/a	N→[Q]→—

Reviewer

Name:

Date:

This is a pseudo-label review, not a diagnosis.

Pipeline version: ecg_inference/five_class_xgb.json | Generated 2026-07-31