



Cell-cycle reversal calibration — vel_scale = 0 vs vel_scale = 2


vel0 forward
mean drift = -0.0002 ± 0.0000
median A_12 = -0.0153 ± 0.0116

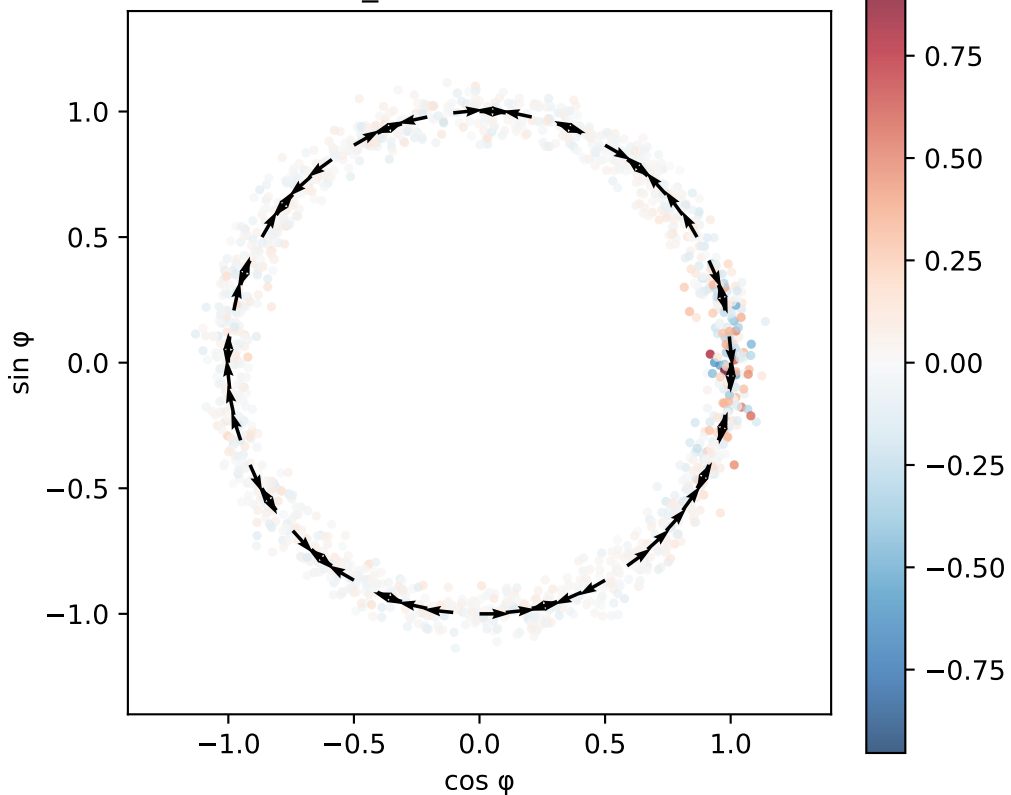

vel0 reverse
mean drift = -0.0002 ± 0.0000
median A_12 = -0.0497 ± 0.0456

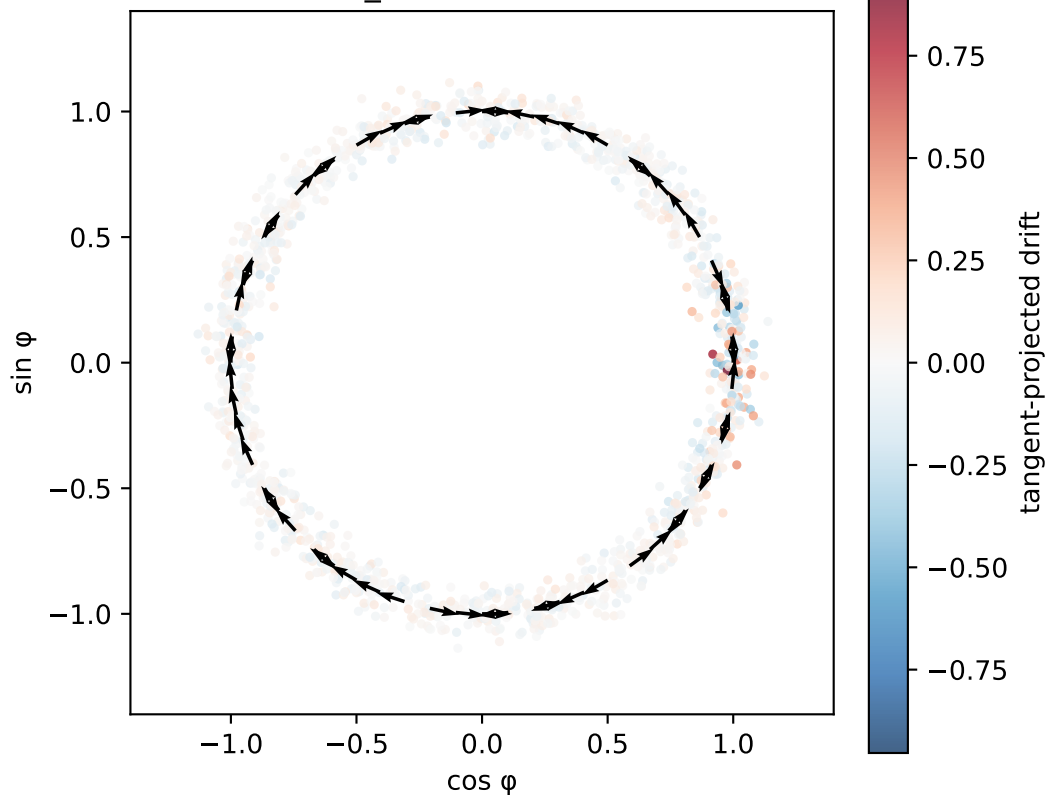

vel2 forward
mean drift = -0.0003 ± 0.0000
median A_12 = $+0.1495 \pm 0.0274$

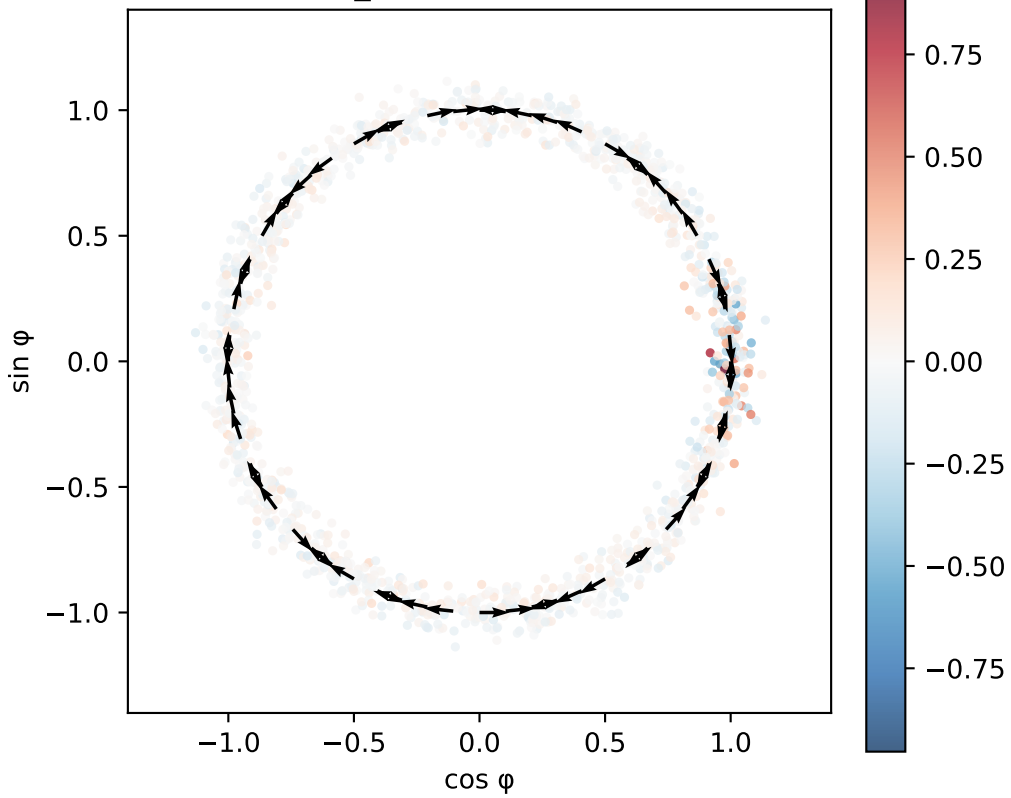

vel2 reverse
mean drift = -0.0001 ± 0.0000
median A_12 = -0.2040 ± 0.0435

