





Title RS-485			Client	Cannot open file C:\Users\Public\Documents\Altium\A
Size: B	Number:2	Revision:1.0	Excellent Benchmark	
Date: 8/29/2017	Time: 1:11:13 PM	Sheet 2 of 9		
File: C:\Users\User\Google Drive\Design Files\Excellent Benchmark Medical Equipment\Medical Gas Alarm\Display Board\RS-485				
5			6	


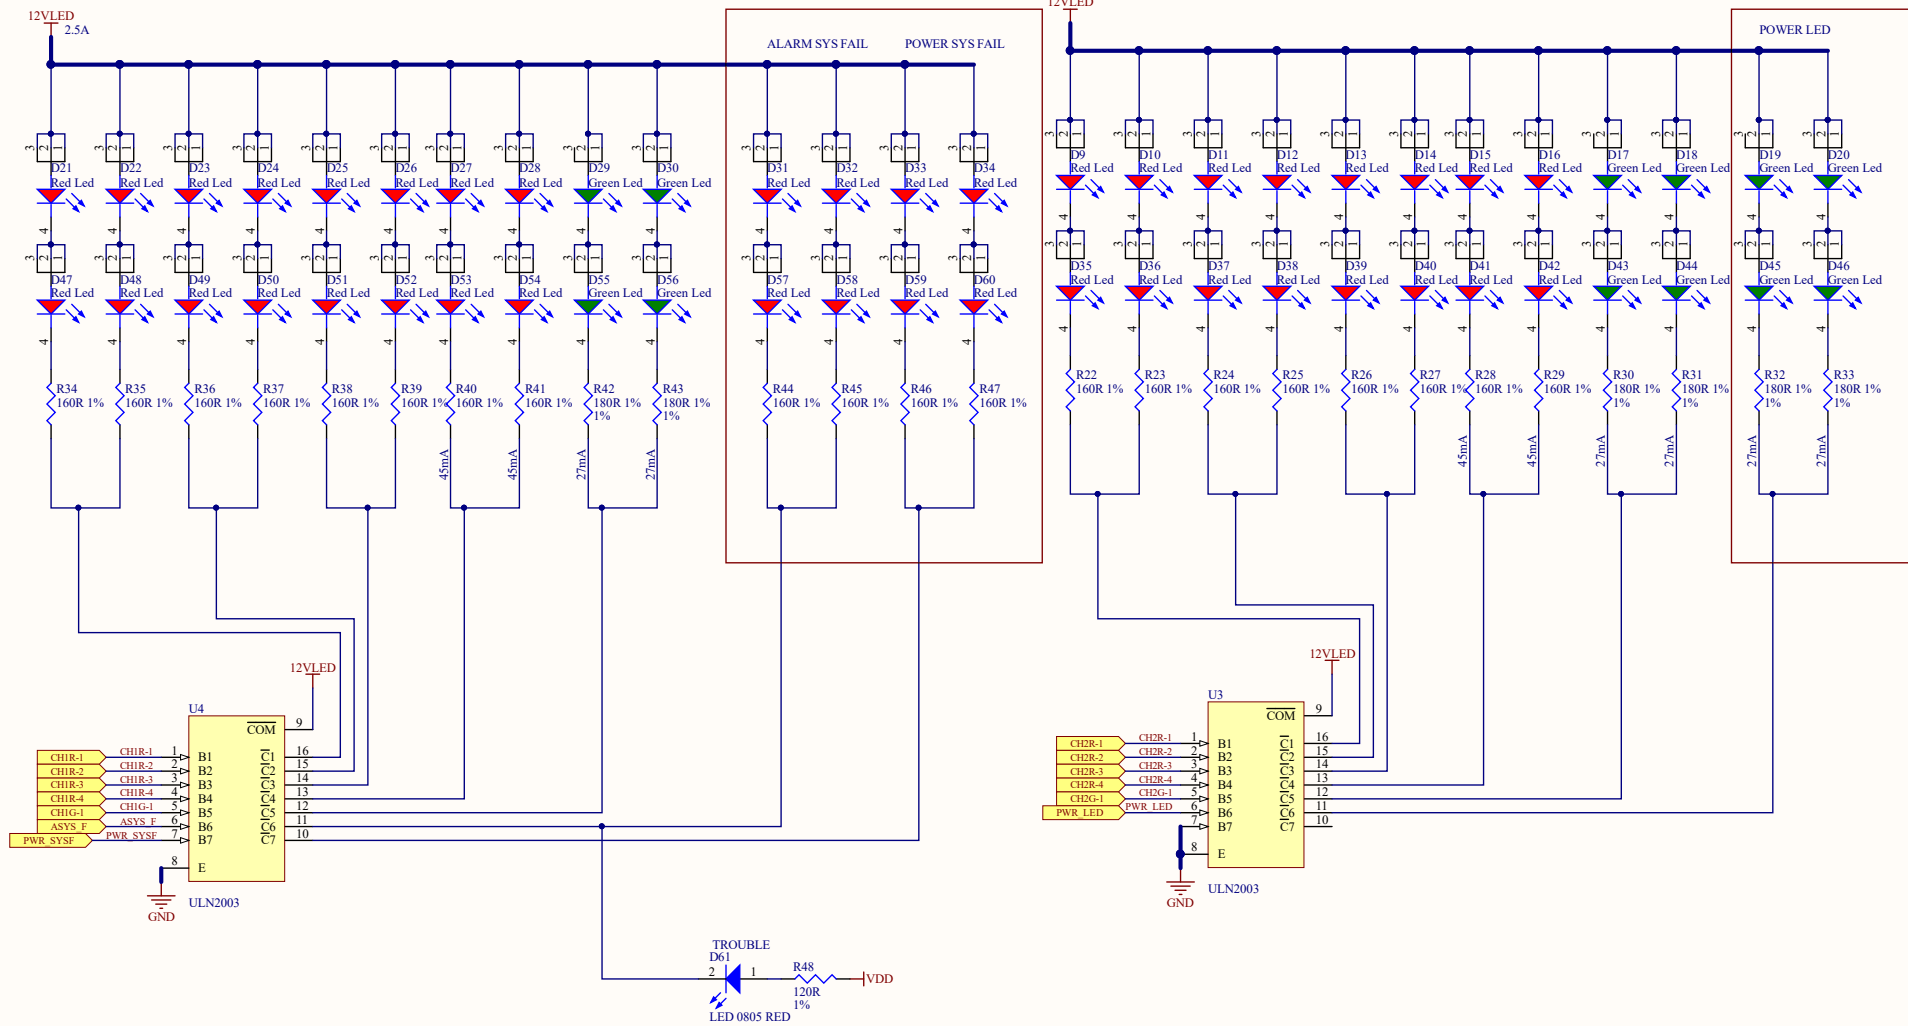


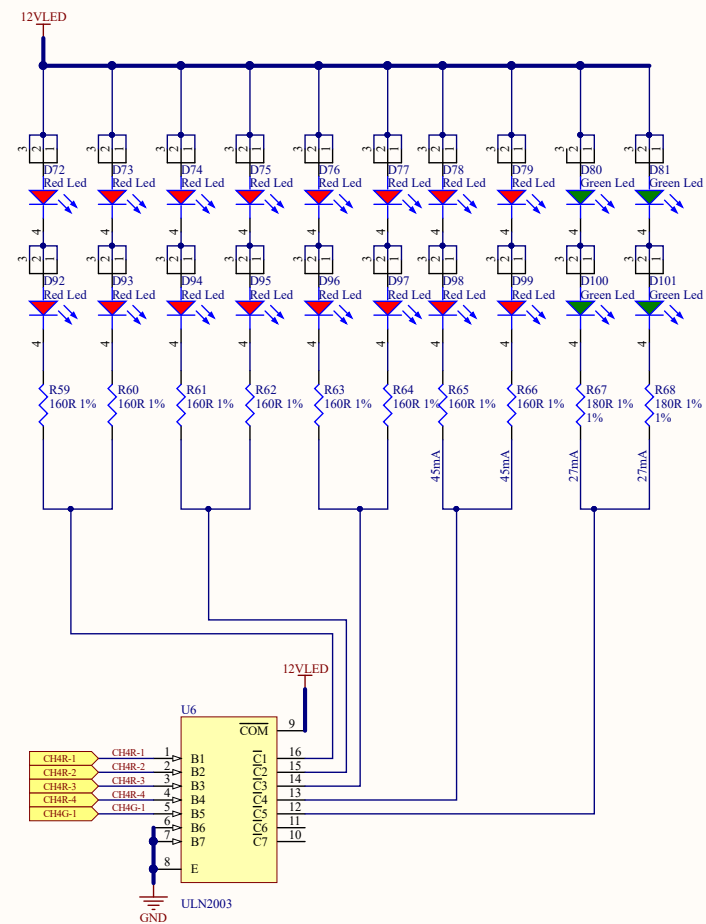




Title OUTPUT CHANNEL 1 TO 2			Client Excellent Benchmark	Cannot open file C:\Users\Public\Documents\Altium\A
Size: B	Number: 4	Revision: 1.0		
Date: 8/29/2017 Time: 1:11:13 PM Sheet 4 of 9				
File: C:\Users\User\Google Drive\Design Files\Excellent Benchmark Medical Equipment\Medical Gas Alarm Display Board\OUTPU				

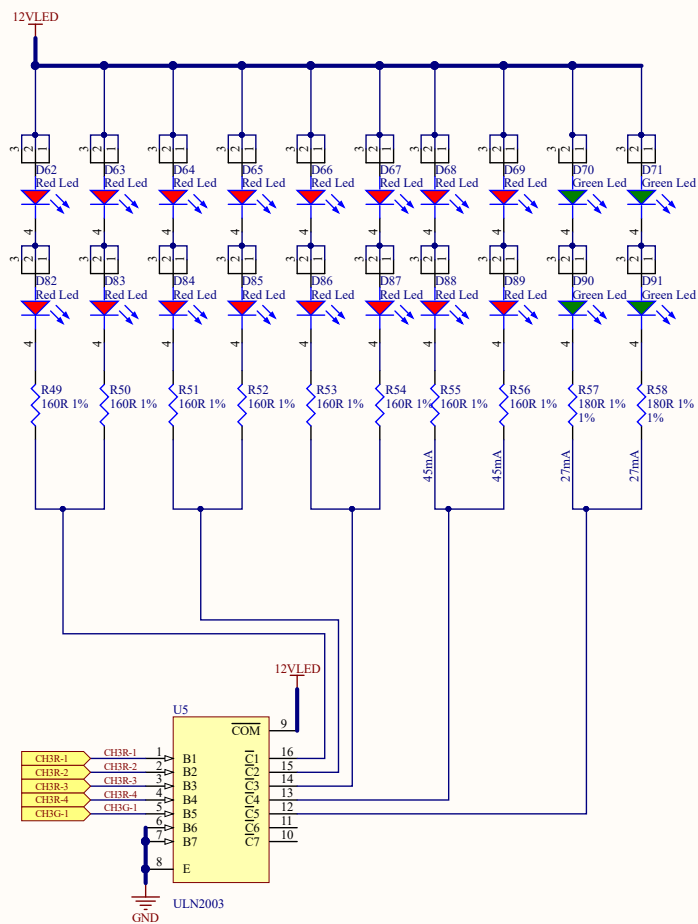

Title OUTPUT CHANNEL 1 TO 2			Client Excellent Benchmark	Cannot open file C:\Users\Public\Documents\Altium\A
Size: B	Number:5	Revision:1.0		
Date: 8/29/2017 Time: 1:11:13 PM Sheet 5 of 9			File: C:\Users\User\Google Drive\Design Files\Excellent Benchmark Medical Equipment\Medical Gas Alarm\Display Board\OUTPU	

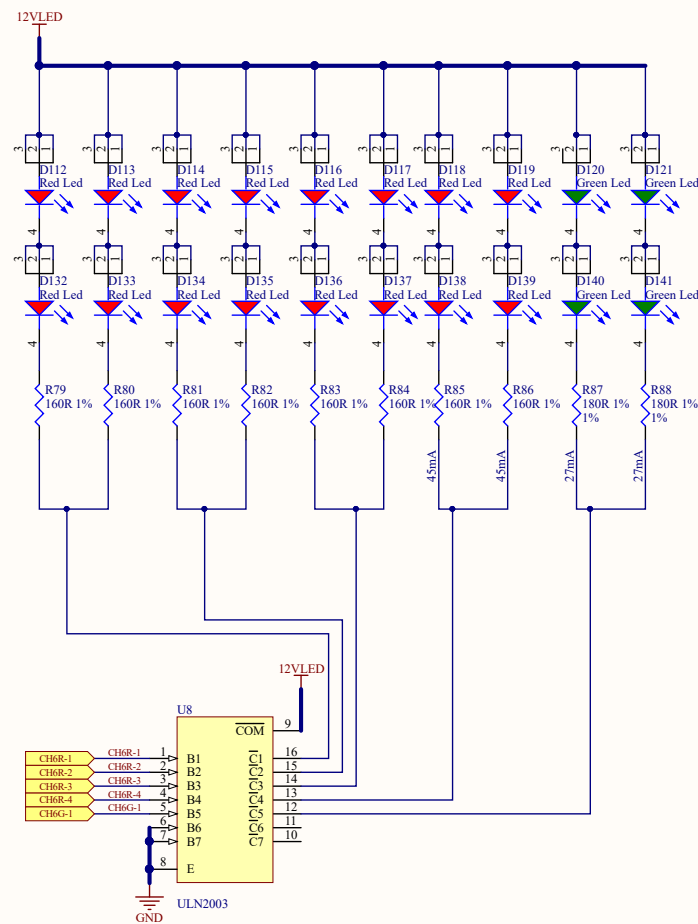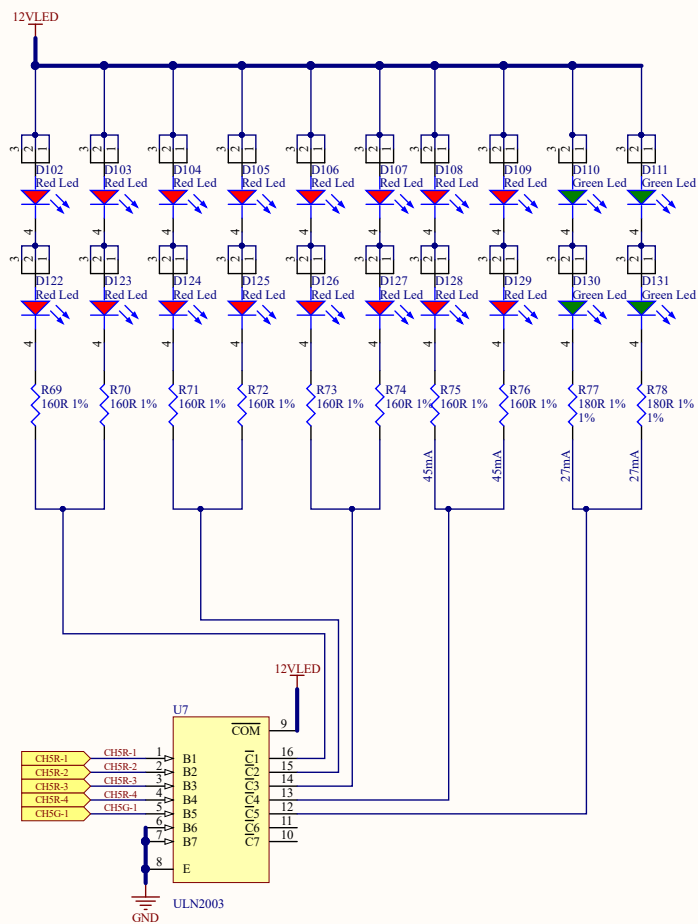


Title OUTPUT CHANNEL 1 TO 2			Client Excellent Benchmark	Cannot open file C:\Users\Public\Documents\Altium\A
Size: B	Number6	Revision:1.0		
Date: 8/29/2017 Time: 1:11:13 PM Sheet 6 of 9				
File: C:\Users\User\Google Drive\Design Files\Excellent Benchmark Medical Equipment\Medical Gas Alarm\Display Board\OUTPU				

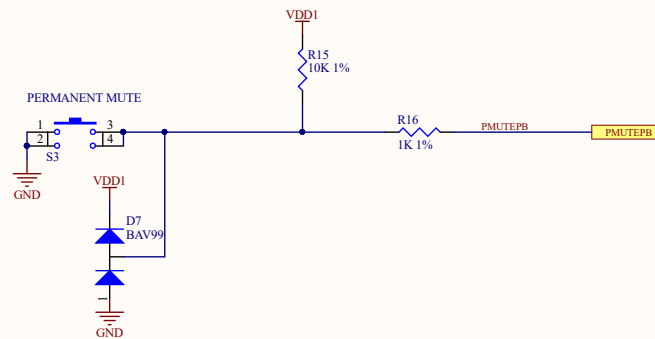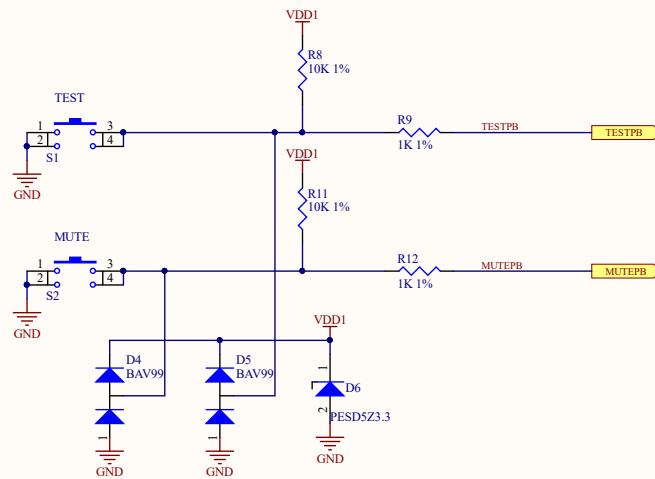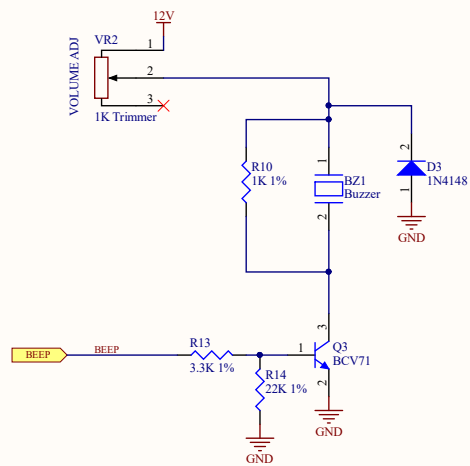


MOUNTING HOLES

M1	M2
3.0mm	3.0mm
M3	M4
3.0mm	3.0mm
M5	M6
3.0mm	3.0mm

Title <i>Extras</i>			Client Excellent Benchmark	Cannot open file C:\Users\Pub lic\Documen ts\Altium\A
Size: B	Number:7	Revision:1.0		
Date: 8/29/2017 Time: 1:11:14 PM Sheet 7 of 9			File: C:\Users\User\Google Drive\Design Files\Excellent Benchmark Medical Equipment Medical Gas Alarm\Display Board\Extras.S	

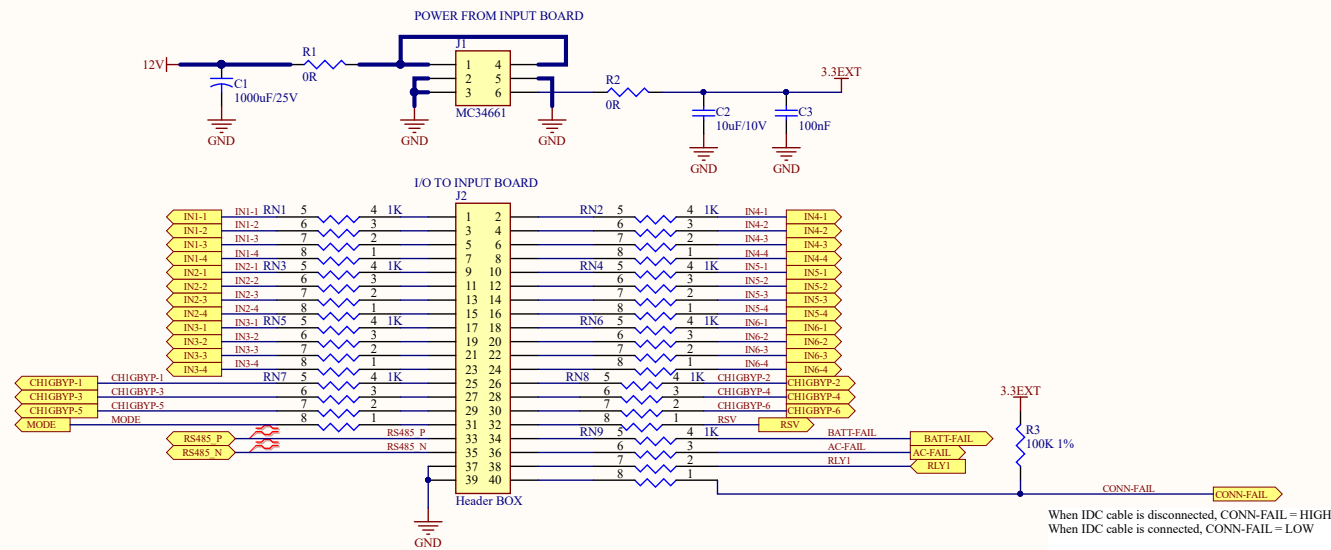

Title CONNECTOR - EXTERNAL			Client Excellent Benchmark	Cannot open file C:\Users\Public\Documents\Altium\A
Size: B	Number: 8	Revision: 1.0		
Date: 8/29/2017	Time: 1:11:14 PM	Sheet: 8 of 9	File: C:\Users\User\Google Drive\Design Files\Excellent Benchmark Medical Equipment\Medical Gas Alarm Display Board\Connect	

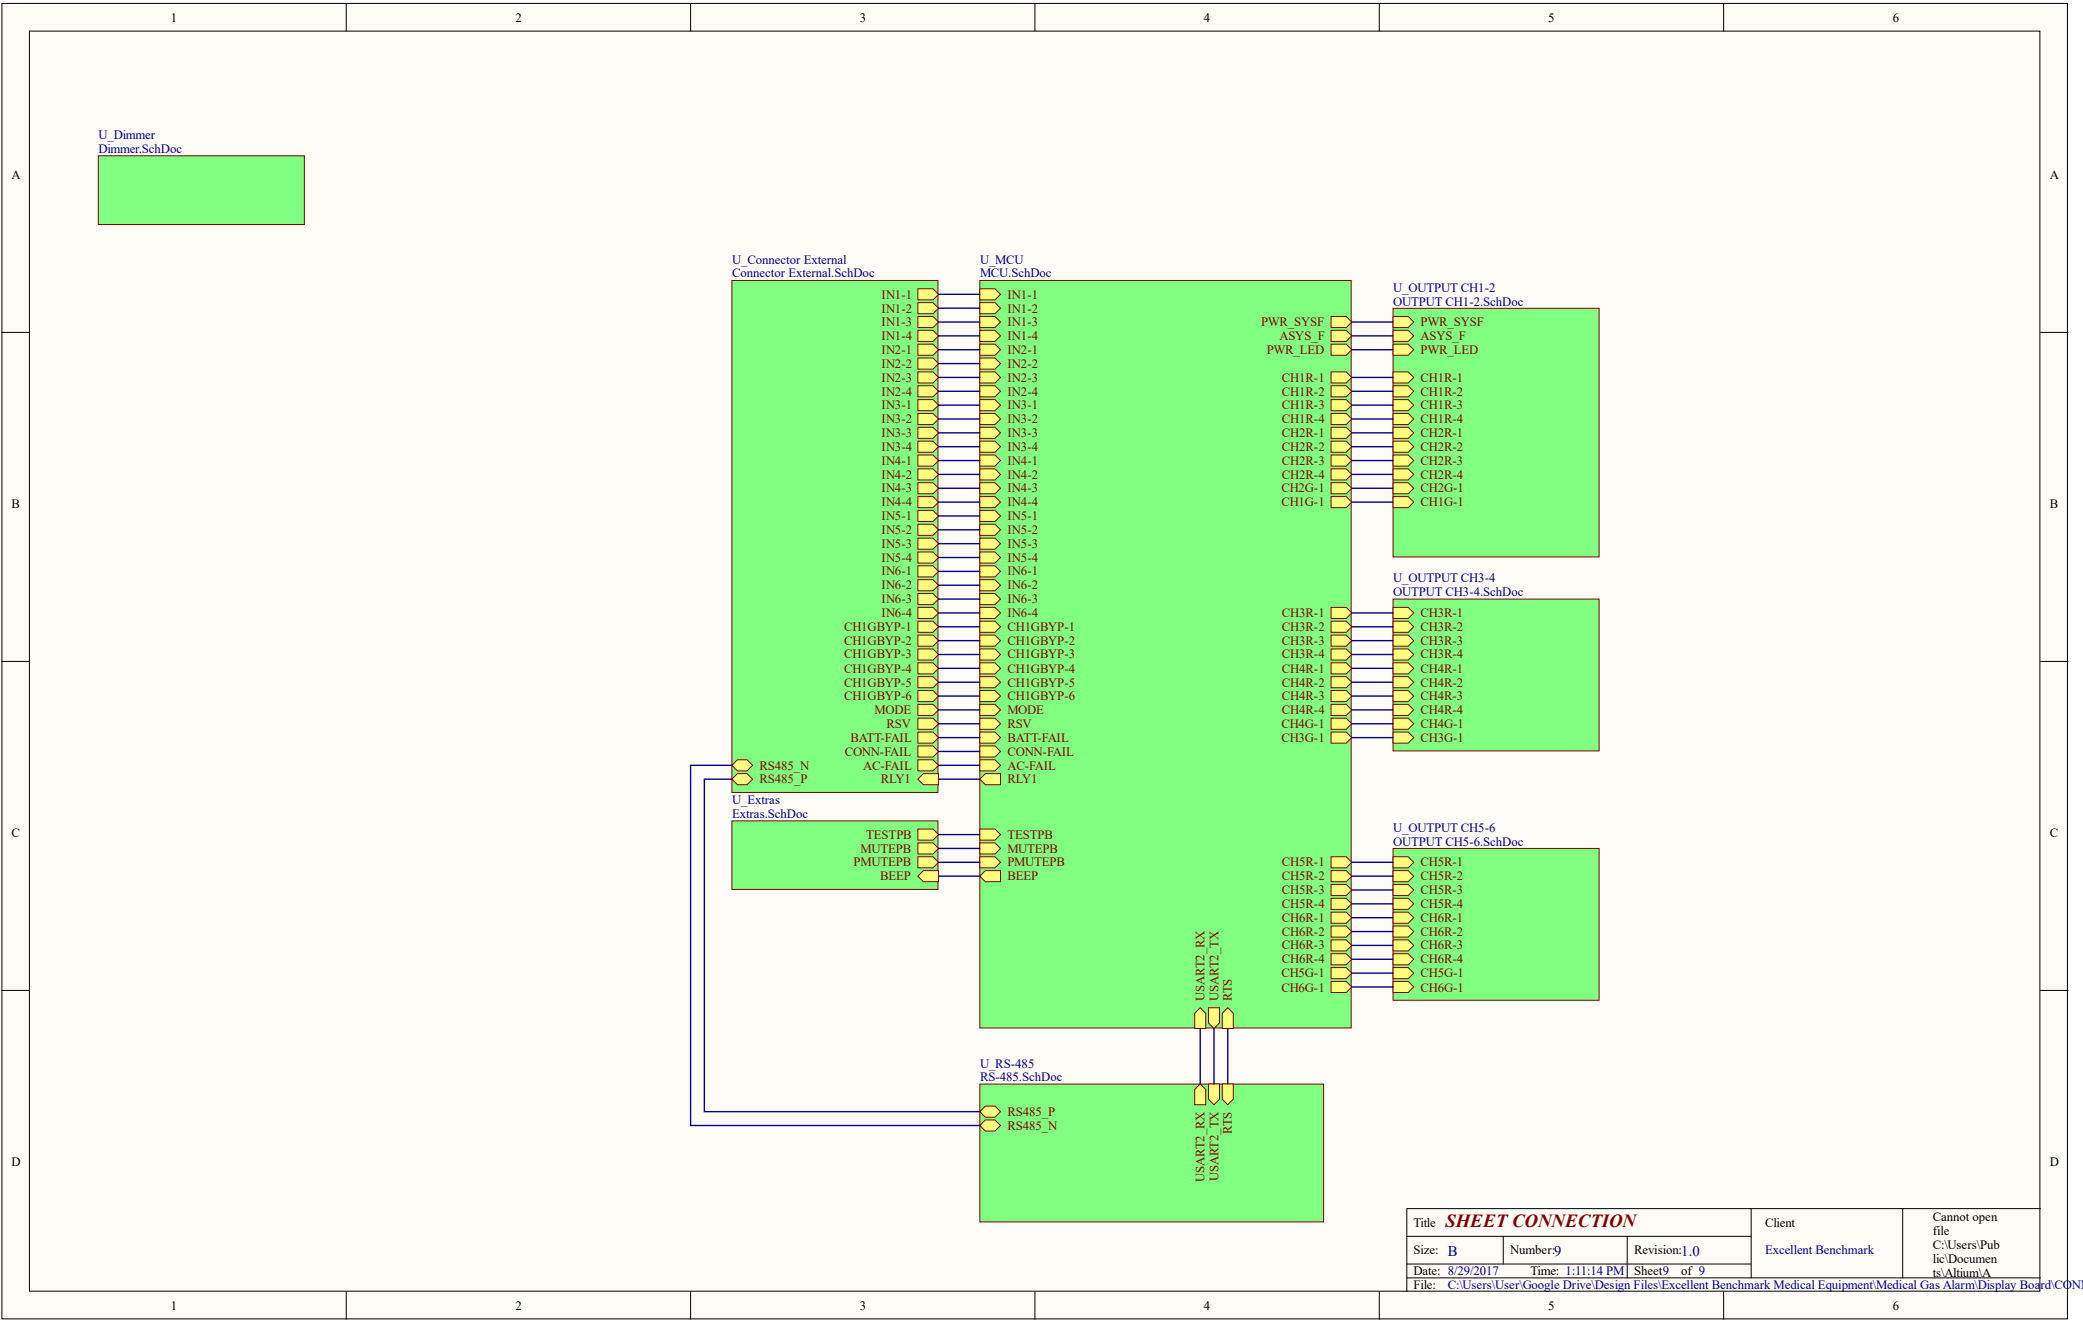

Title <i>SHEET CONNECTION</i>			Client	Cannot open file
Size: B	Number 9	Revision: 1.0	Excellent Benchmark	C:\Users\Public\Documents\Altium\A
Date: 8/29/2017 Time: 1:11:14 PM Sheet 9 of 9				
File: C:\Users\User\Google Drive\Design Files\Excellent Benchmark Medical Equipment\Medical Gas Alarm\Display Board\CON				