


Measurement Details	Measurement Details
Operator Name VLefebur	Analysis Date Time 3/06/2026 10:56:07 AM
Sample Name S1144330_JNJ-16175328-n002-00668 400mg/L 2-8C 3months	Measurement Date Time 3/06/2026 10:56:07 AM
SOP File Name TV-TMD-32593 _ TMC207 micro - PLD for G002.msop	Result Source Measurement
Analysis	Result
Particle Name Polystyrene Latex	Concentration 0.0012 %
Particle Refractive Index 1.610	Span 2.097
Particle Absorption Index 0.010	Uniformity 0.657
Dispersant Name 0.1% Poloxamer 338 in Water	Specific Surface Area 3748 m ² /kg
Dispersant Refractive Index 1.330	D [3,2] 1.60 µm
Scattering Model Mie	D [4,3] 2.80 µm
Analysis Model General Purpose	Dv (10) 0.748 µm
Weighted Residual 0.44 %	Dv (50) 2.25 µm
Laser Obscuration 6.03 %	Dv (90) 5.47 µm

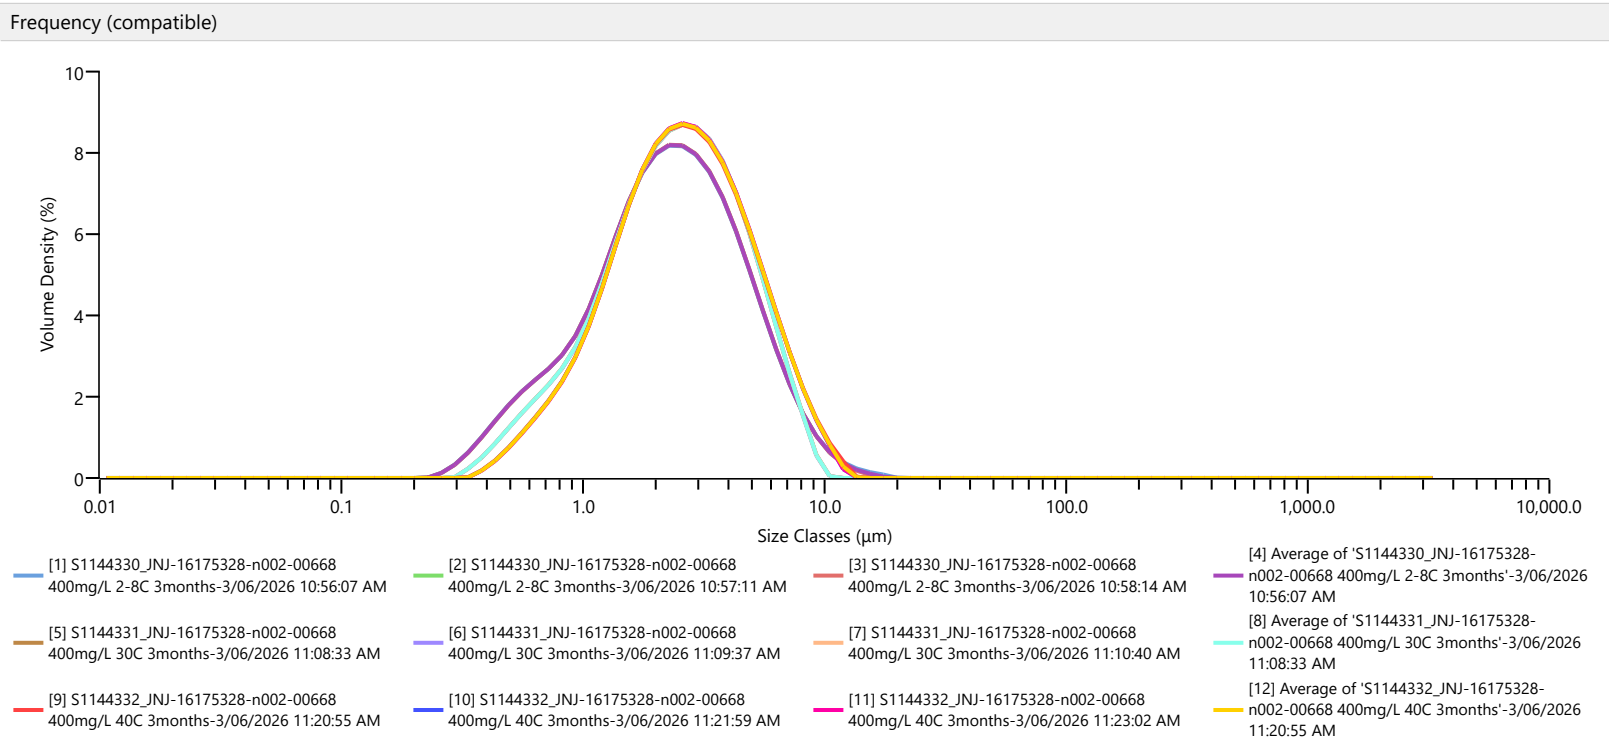

Result															
Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In
0.0100	0.00	0.0463	0.00	0.214	0.00	0.991	3.45	4.58	4.26	21.2	0.00	98.1	0.00	454	0.00
0.0114	0.00	0.0526	0.00	0.243	0.10	1.13	4.16	5.21	3.42	24.1	0.00	111	0.00	516	0.00
0.0129	0.00	0.0597	0.00	0.276	0.27	1.28	4.94	5.92	2.62	27.4	0.00	127	0.00	586	0.00
0.0147	0.00	0.0679	0.00	0.314	0.52	1.45	5.68	6.72	1.91	31.1	0.00	144	0.00	666	0.00
0.0167	0.00	0.0771	0.00	0.357	0.84	1.65	6.28	7.64	1.31	35.3	0.00	163	0.00	756	0.00
0.0189	0.00	0.0876	0.00	0.405	1.18	1.88	6.66	8.68	0.85	40.1	0.00	186	0.00	859	0.00
0.0215	0.00	0.0995	0.00	0.460	1.50	2.13	6.83	9.86	0.53	45.6	0.00	211	0.00	976	0.00
0.0244	0.00	0.113	0.00	0.523	1.78	2.42	6.82	11.2	0.32	51.8	0.00	240	0.00	1110	0.00
0.0278	0.00	0.128	0.00	0.594	2.02	2.75	6.64	12.7	0.19	58.9	0.00	272	0.00	1260	0.00
0.0315	0.00	0.146	0.00	0.675	2.24	3.12	6.29	14.5	0.12	66.9	0.00	310	0.00	1430	0.00
0.0358	0.00	0.166	0.00	0.767	2.51	3.55	5.76	16.4	0.07	76.0	0.00	352	0.00	1630	0.00
0.0407	0.00	0.188	0.00	0.872	2.89	4.03	5.06	18.7	0.00	86.4	0.00	400	0.00	1850	0.00