


Measurement Details	Measurement Details
Operator Name vlefebur	Analysis Date Time 6/05/2026 3:45:44 PM
Sample Name S08662018_400mg/ml 5deg C	Measurement Date Time 6/05/2026 3:45:44 PM
SOP File Name TV-TMD-32593 _ TMC207 micro - PLD for G002.msop	Result Source Measurement
Analysis	Result
Particle Name Polystyrene Latex	Concentration 0.0011 %
Particle Refractive Index 1.610	Span 1.787
Particle Absorption Index 0.010	Uniformity 0.545
Dispersant Name 0.1% Poloxamer 338 in Water	Specific Surface Area 4352 m ² /kg
Dispersant Refractive Index 1.330	D [3,2] 1.38 µm
Scattering Model Mie	D [4,3] 2.09 µm
Analysis Model General Purpose	Dv (10) 0.683 µm
Weighted Residual 0.50 %	Dv (50) 1.81 µm
Laser Obscuration 6.54 %	Dv (90) 3.91 µm

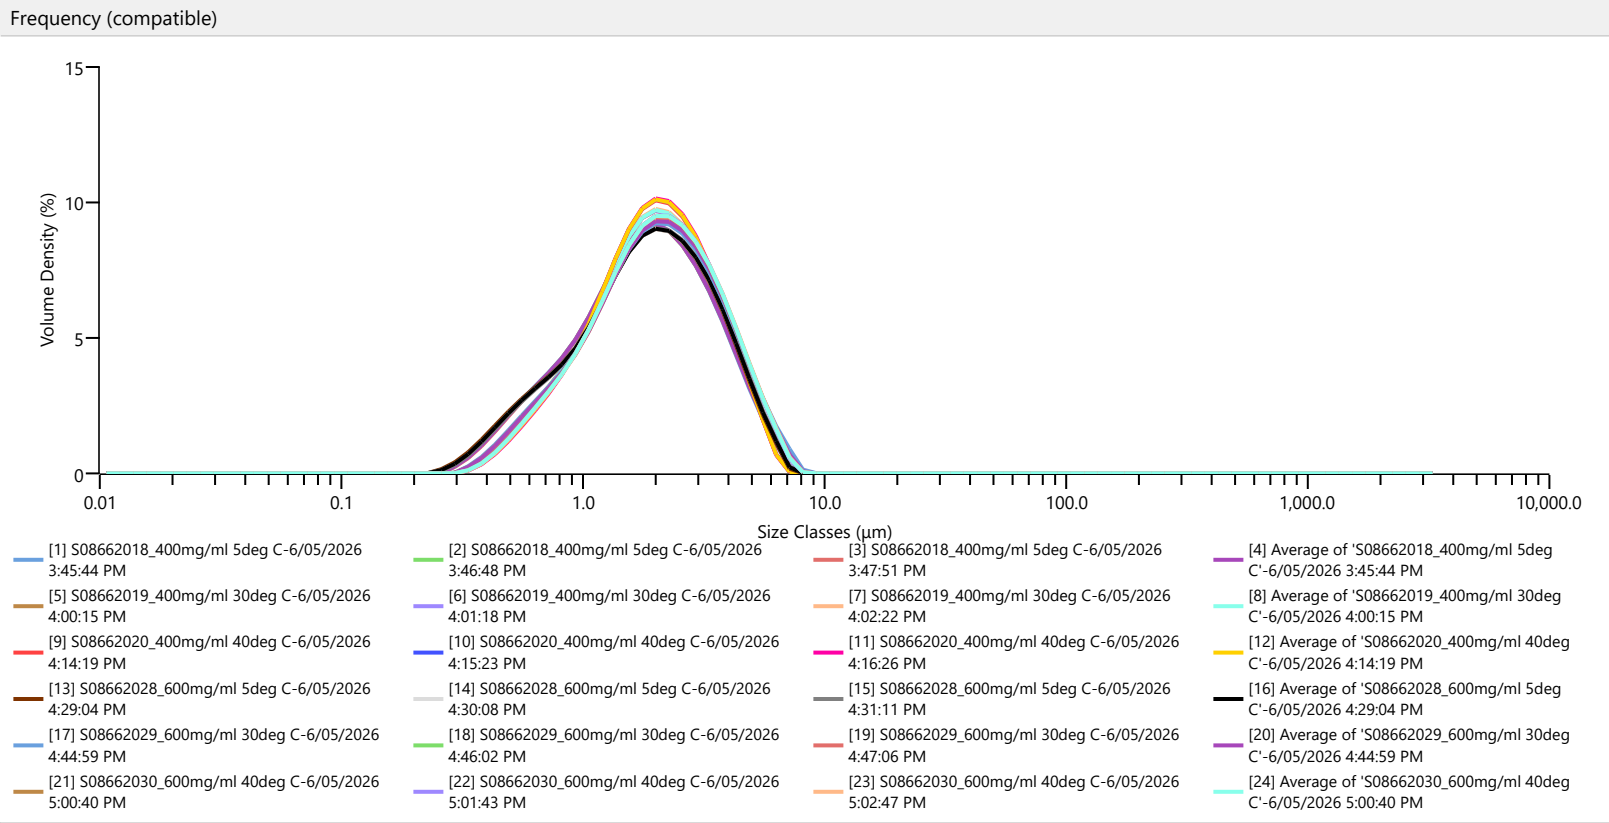

Result															
Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In
0.0100	0.00	0.0463	0.00	0.214	0.00	0.991	4.80	4.58	2.59	21.2	0.00	98.1	0.00	454	0.00
0.0114	0.00	0.0526	0.00	0.243	0.00	1.13	5.63	5.21	1.65	24.1	0.00	111	0.00	516	0.00
0.0129	0.00	0.0597	0.00	0.276	0.22	1.28	6.48	5.92	0.89	27.4	0.00	127	0.00	586	0.00
0.0147	0.00	0.0679	0.00	0.314	0.50	1.45	7.19	6.72	0.14	31.1	0.00	144	0.00	666	0.00
0.0167	0.00	0.0771	0.00	0.357	0.89	1.65	7.62	7.64	0.00	35.3	0.00	163	0.00	756	0.00
0.0189	0.00	0.0876	0.00	0.405	1.34	1.88	7.71	8.68	0.00	40.1	0.00	186	0.00	859	0.00
0.0215	0.00	0.0995	0.00	0.460	1.81	2.13	7.49	9.86	0.00	45.6	0.00	211	0.00	976	0.00
0.0244	0.00	0.113	0.00	0.523	2.26	2.42	7.03	11.2	0.00	51.8	0.00	240	0.00	1110	0.00
0.0278	0.00	0.128	0.00	0.594	2.69	2.75	6.40	12.7	0.00	58.9	0.00	272	0.00	1260	0.00
0.0315	0.00	0.146	0.00	0.675	3.10	3.12	5.61	14.5	0.00	66.9	0.00	310	0.00	1430	0.00