


Measurement Details	Measurement Details
Operator Name MAShtika	Analysis Date Time 12/02/2026 10:25:01 AM
Sample Name S1144326 - 400 mg/mL microsuspension T0	Measurement Date Time 12/02/2026 10:25:01 AM
SOP File Name TV-TMD-32593 _ TMC207 micro - PLD for G002.msop	Result Source Measurement
Analysis	Result
Particle Name Polystyrene Latex	Concentration 0.0015 %
Particle Refractive Index 1.610	Span 2.090
Particle Absorption Index 0.010	Uniformity 0.648
Dispersant Name 0.1% Poloxamer 338 in Water	Specific Surface Area 3679 m ² /kg
Dispersant Refractive Index 1.330	D [3,2] 1.63 µm
Scattering Model Mie	D [4,3] 2.76 µm
Analysis Model General Purpose	Dv (10) 0.766 µm
Weighted Residual 0.51 %	Dv (50) 2.24 µm
Laser Obscuration 7.34 %	Dv (90) 5.45 µm

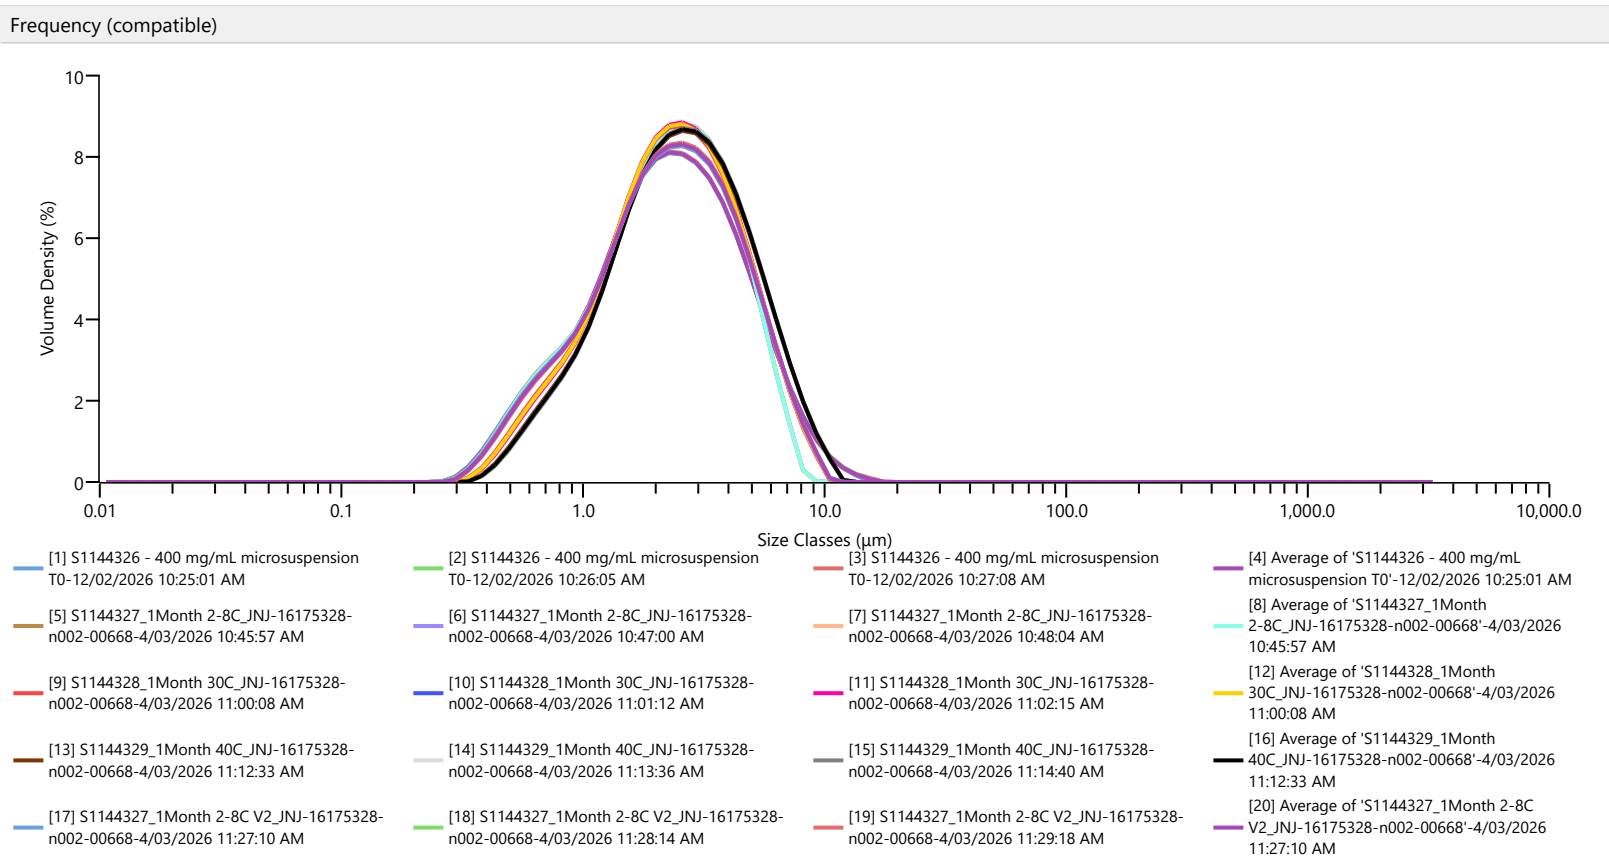

Result															
Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In	Size (µm)	% Volume In
0.0100	0.00	0.0463	0.00	0.214	0.00	0.991	3.60	4.58	4.30	21.2	0.00	98.1	0.00	454	0.00
0.0114	0.00	0.0526	0.00	0.243	0.00	1.13	4.26	5.21	3.48	24.1	0.00	111	0.00	516	0.00
0.0129	0.00	0.0597	0.00	0.276	0.10	1.28	5.02	5.92	2.68	27.4	0.00	127	0.00	586	0.00
0.0147	0.00	0.0679	0.00	0.314	0.31	1.45	5.73	6.72	1.96	31.1	0.00	144	0.00	666	0.00
0.0167	0.00	0.0771	0.00	0.357	0.64	1.65	6.29	7.64	1.34	35.3	0.00	163	0.00	756	0.00
0.0189	0.00	0.0876	0.00	0.405	1.04	1.88	6.63	8.68	0.86	40.1	0.00	186	0.00	859	0.00
0.0215	0.00	0.0995	0.00	0.460	1.46	2.13	6.76	9.86	0.51	45.6	0.00	211	0.00	976	0.00
0.0244	0.00	0.113	0.00	0.523	1.85	2.42	6.73	11.2	0.27	51.8	0.00	240	0.00	1110	0.00
0.0278	0.00	0.128	0.00	0.594	2.18	2.75	6.56	12.7	0.12	58.9	0.00	272	0.00	1260	0.00