

UE LABS Presentation


NURIA BAS

UE CS&Q Director & Labs Director

Life Is On

Schneider
Electric

UE Laboratories Introduction

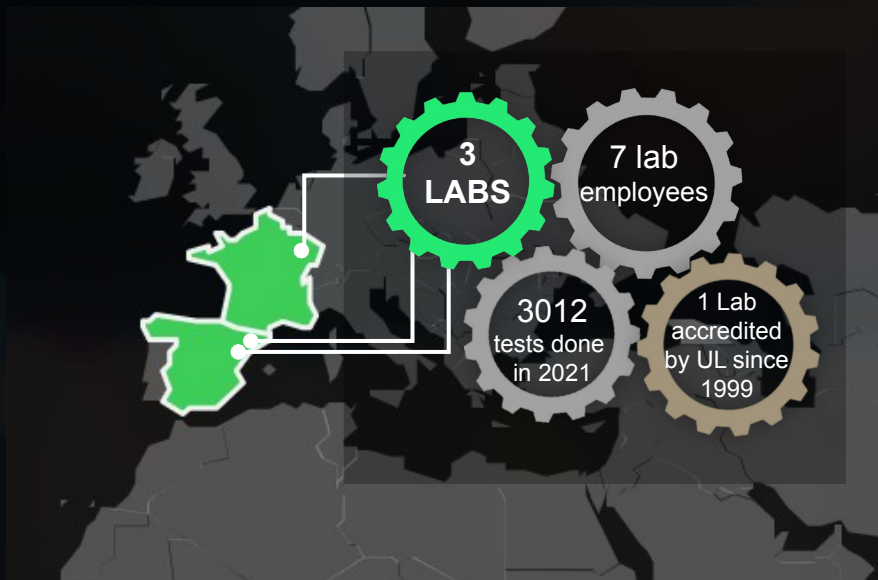

3

Labs

7 Lab

Employees


One lab in each manufacturing plant. Sarre Union, Molins de Rei & Capellades.

**1 Lab
Accredited
by UL**

5 lab technicians, 1 Test & Expert Leader and Lab Manager.

Capellades Lab is CTDTP (Client Test Data Program) by UL since 1999, with a File number DA307.

SE Organization Chart

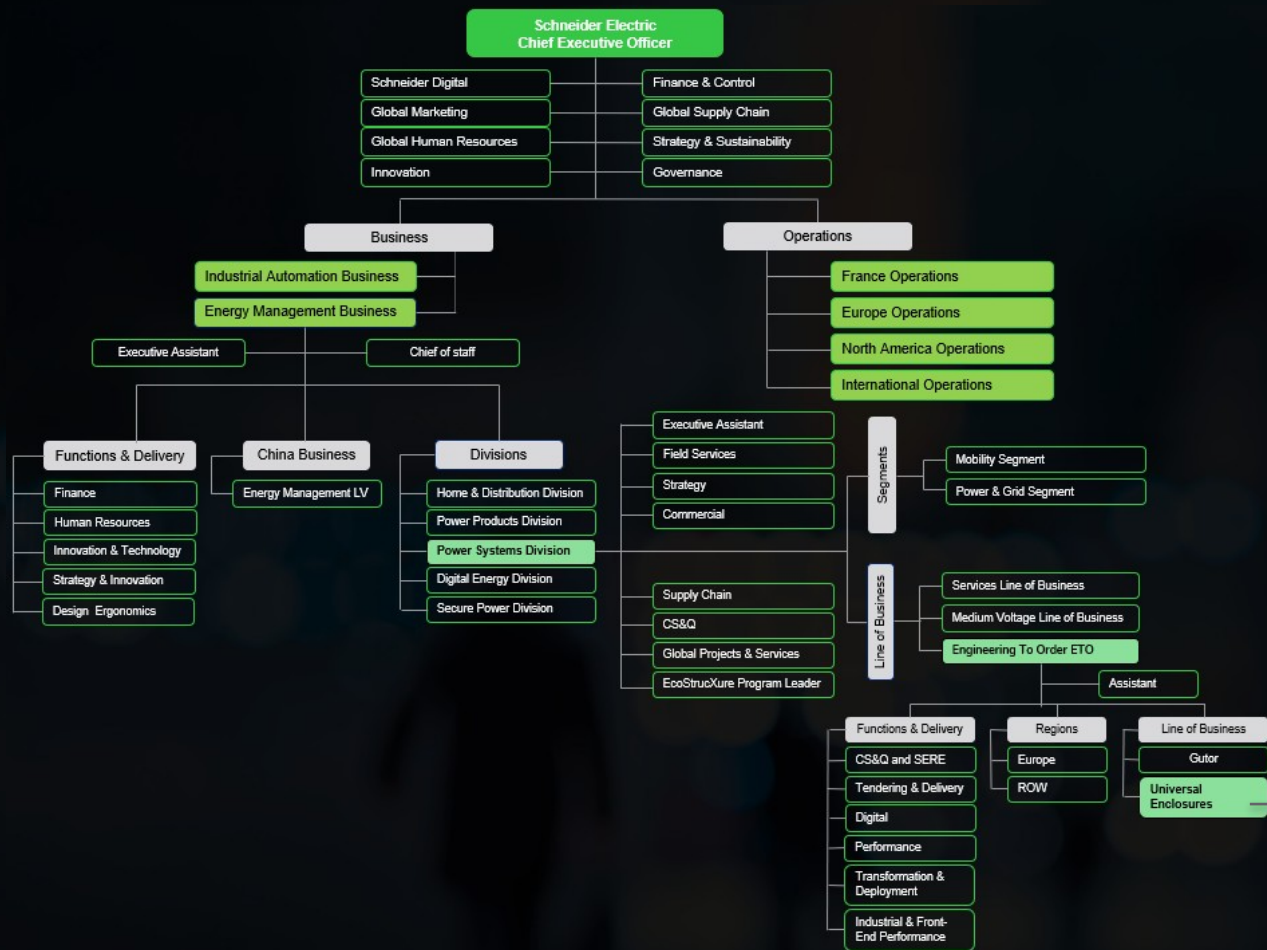


UNIVERSAL ENCLOSURES
LoB is inside:

Energy
Management
Business

Power Systems &
services Division

ETO (Engineering
To Order) LoB

Universal Enclosures Organization Chart

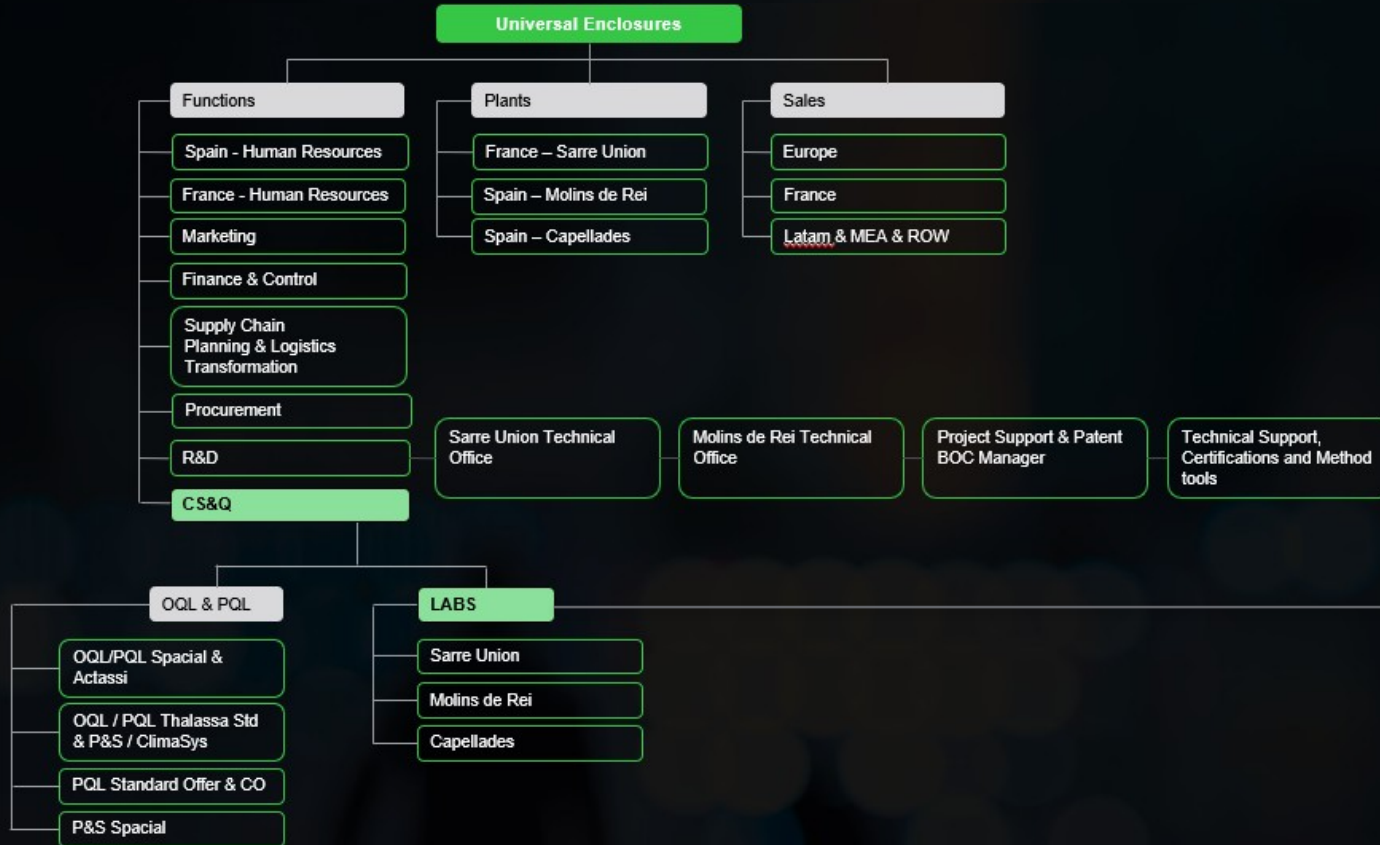


**UNIVERSAL
ENCLOSURES**
LAB is inside

Customer
Satisfaction &
Quality
Department

Lab is lead
directly by the
CS&Q Director


UE LABS Organization Chart

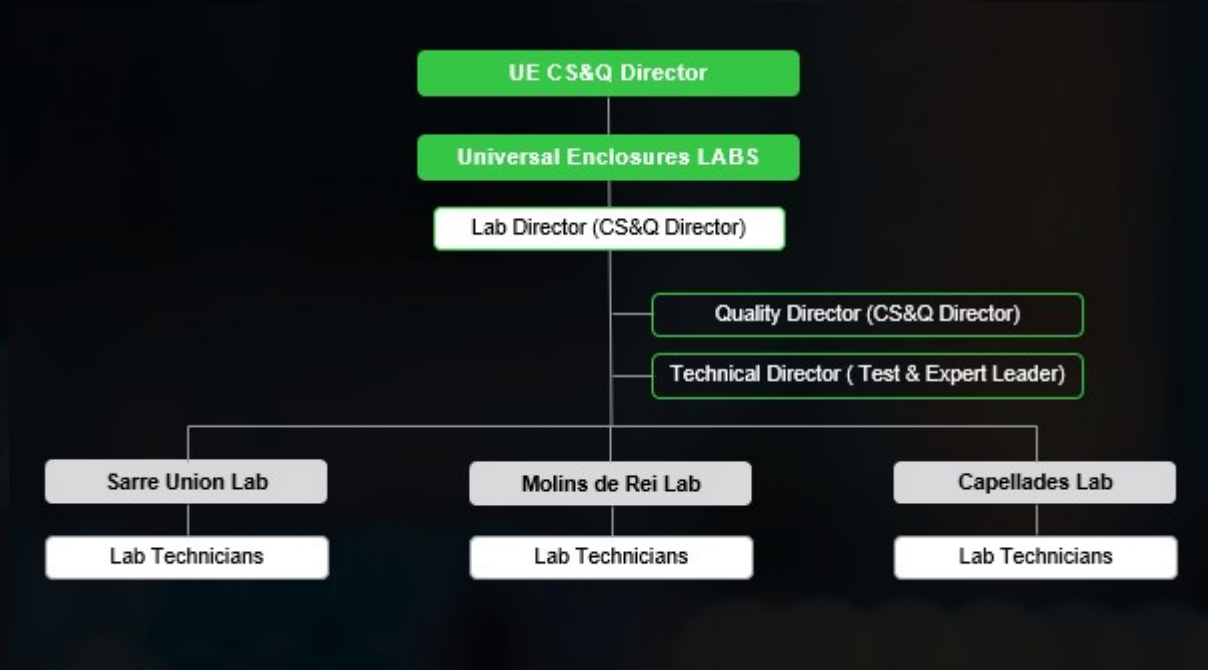

CS&Q Director is leading directly UE labs and as well as the function of Quality Director for the labs.

The Technical Director for labs is what we call internally “Test & Expert Leader”.

Our Mission

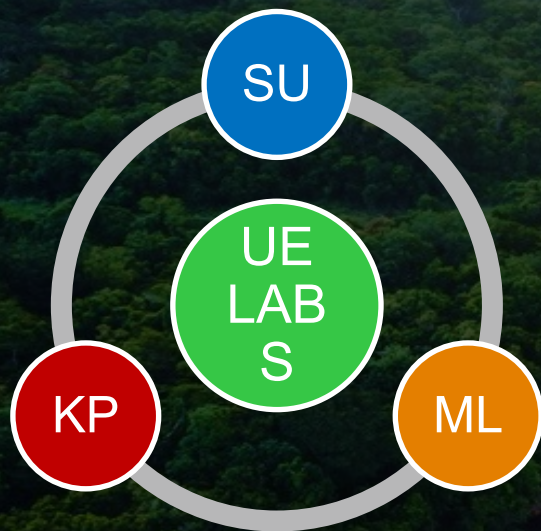


SU: Sarre-Union Lab (France)
ML: Molins de Rei Lab (Spain)
KP: Capellades Lab (Spain)

- Assure the quality of the standard of production
- Ensure qualification of product evolutions or new products launch
- Ensure certifications tests (1 UL accredited Lab)
- Validate P&S specific solutions
- Analyse returns (RTA and TEX)
- Give support to the Customer Technical Support team
- Manage the calibration of labs & plants equipment

Capellades Lab



Sarre-Union Lab

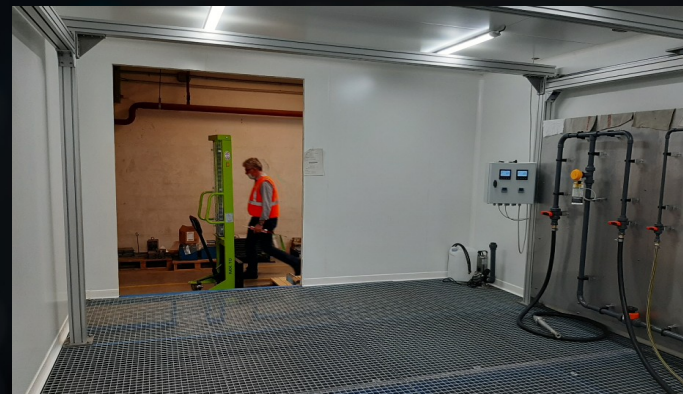

Molins de Rei Lab



Standards



Capellades Lab is CTDP (Client Test Data Program) by UL since 1999, with a File number DA307. We can do the tests according to UL Standard with total autonomy and direct recognition of Underwriters Laboratories Inc.

IEC 62208

Empty enclosures for low-voltage switchgear and controlgear assemblies - General requirements

ISO 12944-6

Paints and varnishes — Corrosion protection of steel structures by protective paint systems — Part 6: Laboratory performance test methods

UL 50 / CSA C22.2 N° 94.1

Enclosures for Electrical Equipment, Non-Environmental Considerations

UL 50E / CSA C22.2N° 94.2

Enclosures for Electrical Equipment, Environmental Considerations

UL 746 C

Standard for Polymeric Materials - Use in Electrical Equipment Evaluations

IEC 62208

Empty enclosures for low-voltage switchgear and controlgear assemblies - General requirements

ISO 12944-6

Paints and varnishes — Corrosion protection of steel structures by protective paint systems — Part 6: Laboratory performance test methods

ISO 4624


Paints and varnishes — Pull-off test for adhesion

IEC 60079-0

Explosive atmospheres -- Part 0: Equipment - General requirements

EN 61386-1

Conduit systems for cable management -- Part 1: General requirements

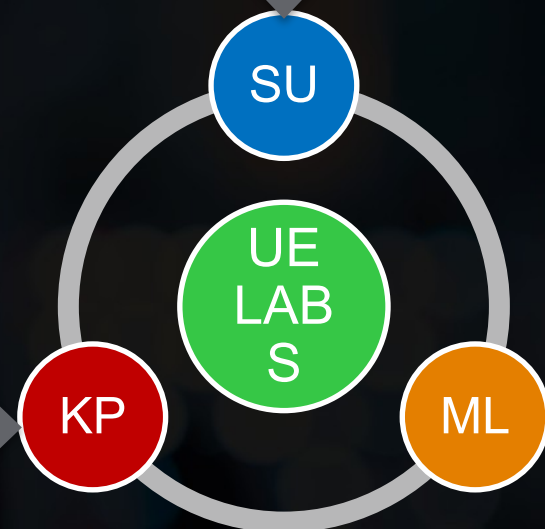

IEC 62208

Empty enclosures for low-voltage switchgear and controlgear assemblies - General requirements

IEC 61439-1

Low-voltage switchgear and controlgear assemblies - Part 1: General rules

IEC 61439-5

Low-voltage switchgear and controlgear assemblies - Part 5: Assemblies for power distribution in public networks

Types of Products Tested

Spacial, Thalassa, and ClimaSys



Types of Products Tested



Spacial

Steel and stainless steel



Thalassa

Plastic and glass-reinforced polyester



ClimaSys

Thermal management systems

Life Is On

