	Environmental Analysis Teaching and Research Laboratory	Date: 1/27/2024	SOP No. 37b v0.92
	Standard Operating Procedure	Title: Compost Maturity	
	Approved By: Los Huertos	Revised: January 28, 2024	

1. Scope and Application

1.1 The Solvita Compost Maturity Test is a unique procedure using two test probes to simultaneously measure CO₂ and NH₃, the two most prominent gases indicating activity and stability of compost.

1.2 This test is widely-recognized worldwide for validating compost maturity.

1.3 This easy-to-use application requires a small sample placed in the incubation jars and the results are read after 4-hrs of exposure. The basic kit offers a Solvita color chart to determine the level of activity from which a Maturity Index is calculated using guidelines provided in the manual.

1.4

1.5 Numerous studies... ([Vargas et al., 2005](#)).

2. Acknowledgements

2.1 This SOP is based on the Solvita Field Test Kit Manual ([Solvita, 2014](#)), version 8.

3. Definitions

Compost Compost is a mixture of organic residues that have been piled, watered, and have undergone thermophilic and mesophilic decomposition.

Compost Maturity Compost maturity is the degree of stability of the compost product and the degree to which it is free of phytotoxic (plant-toxic) compounds. Figure 1 shows the relationship between compost maturity and the composting process.

Maturity Index The Maturity Index is a numerical value that is calculated from the CO₂ and NH₃ readings. The Maturity Index is a relative measure of the degree of stability of the compost. The higher the Maturity Index, the more stable the compost. The Maturity Index is calculated using the following formula:

4. Biases and Interferences

4.1 Biases and interferences can come from...

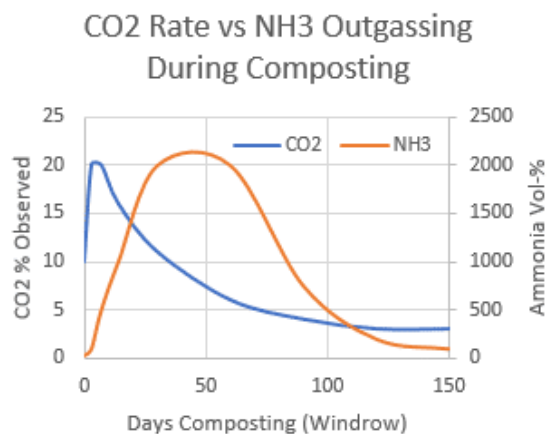


Figure 1: Compost Maturity

5. Health and Safety**6. Personnel & Training Responsibilities**

Students using this SOP should be trained for the following SOPsa:

- SOP1
- SOP2

7. Required Materials

- Test Soils
- # XX Sieves (3/8" or 10 mm)
- Solvita Jars
- Individually wrapped CO₂ & NH₃ Probes (must remain refrigerated)
- DCR Field Test Unit (with 9 volt battery)
- AWS digital scale (field) or Ohaus digital scale (lab)

8. Estimated Time

8.1 This will take 20 minutes to collect and prepare compost sample. An equilibrium stage ranges from 1 to 24 hours depending on conditions. The incubation requires 4 hours. Finally, an additional 10 minutes is needed to read the probes for a total of 5.5 to 28.5 hours.

9. Sample Collection, Preservation, and Storage

Obtain and Prepare Sample

- 9.1** Take several grab samples to prepare a compost by mixing all sub-samples representative of the entire compost. Remove large weed chips and other objects. A 3/8" (10 mm) sieve is recommended before loading jar.
- 9.2** Check moisture content of sample using squeeze test. Squeeze a handful of compost and release. Water should appear between fingers, but not drip out. Adjust water content if needed. Allow compost to equilibrate for 24 hours.
- 9.3** If compost is warm or frozen, let it equilibrate to room temperature for 24 hours before testing.

10. Procedure

- 10.1** Sieve compost to remove large particles.
- 10.2** Carefully fill the Solvita jar to the fill lines. To get the proper density tap the jar gently while filling to fill line. Optionally, the proper weight in grams per jar corresponding to actual field density is found in the Table 1.

Table 1: Compost weight per jar adjusted for actual field density.

lbs/yr ³	kg/m ³	g/jar
500	300	30
800	475	50
1,000	600	60
1,200	700	70

- 10.3** Let the sample "air-out" briefly in the jar for up to one-hour prior to starting the test. If the sample was taken directly from a very hot or frozen pile, it is advisable to allow it to stand for 24 hours before starting the test.
- 10.4** The Solvita maturity method requires two tests carried out simultaneously in the same 4-hour period. Terr open both the pouches marked "High CO₂" and "Ammonia" and carefully remove each probe and avoid touching the gel surface. The gel in the probe is color-coded: the carbon dioxide probe is purple and the ammonia probe is yellow. Once the pouch is open, the test should be started immediately.
- 10.5** Carefully insert both probes into the compost without allowing compost to touch the gel surface. Push the probes so the bottom of the probe hits the jar's bottom. Do not jostle the composite or allow dust to coat the surface of the probe.

10.6 Screw on lid tightly and allow to incubate out of direct sunlight – and wait 4 hours. Record temperature and try to keep the jars at a constant temp for the duration of the test, between 20-25°C (68-77°F).

10.7 Remove lid after 4 hours and remove the probes.

10.8 Read the probes immediately after removing from the jar.

Reading the Results

10.9 Turn on DCR Field test unit and insert probe to get CO₂ and NH₃ color. The probe must go into the DCR with gel side up press the read button.

10.10 Insert the NH₃ probe into the DCR and press the read button. Compare color to the visual color key. Record the NH₃ reading.

10.11 If the DCR does not work, Compare the color of the gel to the color chart, finding the closest match. Record the CO₂ and NH₃ readings.

Clean Up

10.12 Discard compost sample and probe in an appropriate manner.

10.13 Wash the Solvita jar with water and dry for reuse. Label jar top with event to track the number of times the jar has been used. Discard the jar after 4 uses.

11. Data Analysis and Calculations

11.1 Calculate the maturity index using the following formula:

$$MI = \frac{CO_2 \times 0.5 + NH_3 \times 0.5}{100} \quad (1)$$

Compost Maturity Index

11.2 See Figure! 1 below for interpretation:

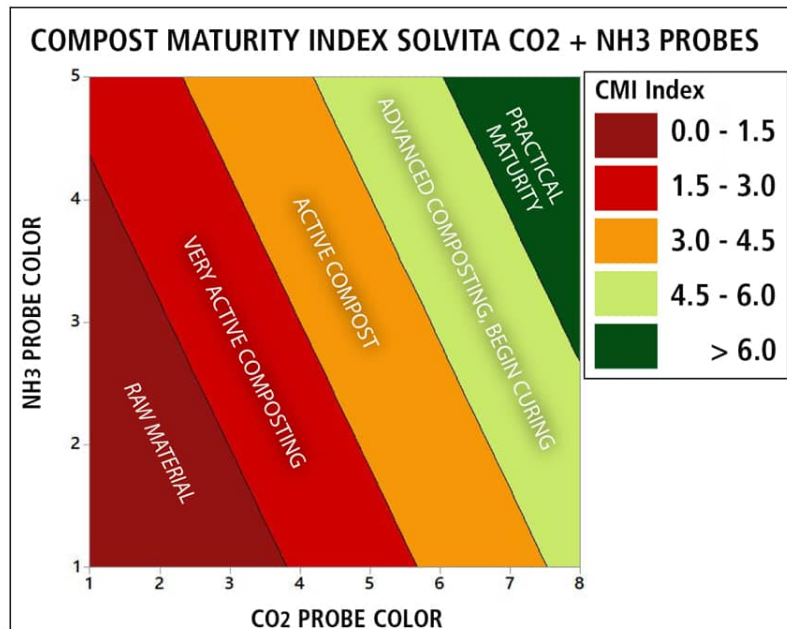


Figure 2: Interpretation of compost maturity index.

12. Applications of Results

Status and Conditions of Compost Processes

Managing Aeration Sufficiency

Selecting Best Use of Composed Based on Maturity

Ammonia Emissions of Mantures & Composts

13. QC/QA Criteria

13.1 The probe show Lot No. and Expiration Dates on the package. Solvita kits are pre-calibrated and packaged for the highest quality prior to shipping. The sealed probes should be the "Control Color" when the foil pack is opened (see color chart). Shelf-life is improved by refrigeration. Do not allow gels to freeze.

13.2 The plastic jars may be reused 4 times, the discarded.

13.3 If the foil packs are damaged or the jar is cracked then the test may not work properly.

13.4 A sample that is too dry may give a false positive maturity test (although goty

ammonia is still volatile).

14. Trouble Shooting

Table 2: Trouble Shooting Guide

Problem	Cause	Solution
Compost is fresh but test results indicate “mature”	Compost is too dry	Add water to compost and retest

15. References

References

- Solvita, L. (2014). *Official Solvita Guideline: Compost Emissions Test: A New Tool for Compost Maturity Assessment*.
- Vargas, D. C., Monedero, M. S., Urpilainen, S., Kamilaki, A., and Stentiford, E. (2005). Assessing the stability and maturity of compost at large-scale plants. *Ingeniería*, 9(2):25–30.