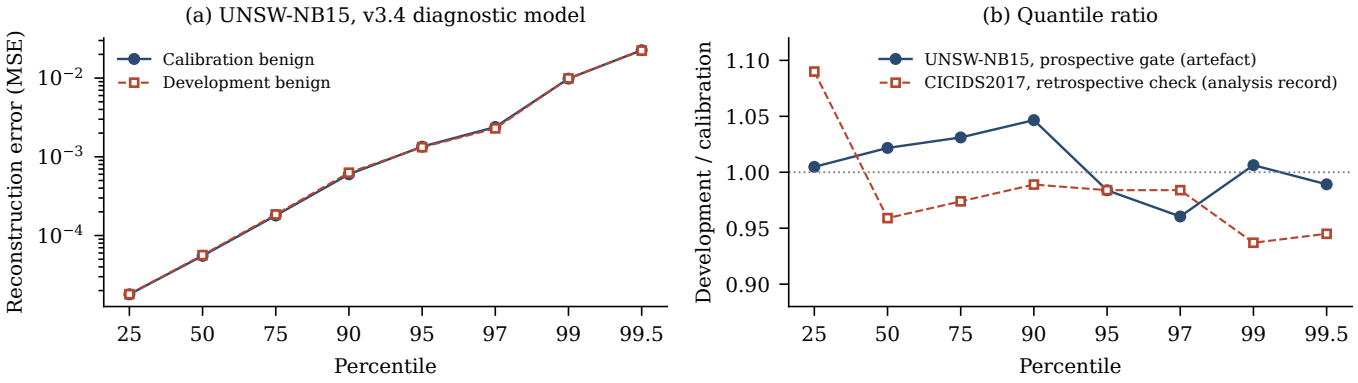
(a) UNSW-NB15, v3.4 diagnostic model
Calibration benign
Development benign
Reconstruction error (MSE)
10^{-2}
10^{-3}
10^{-4}
25
50
75
90
95
97
99
99.5
Percentile
(b) Quantile ratio
UNSW-NB15, prospective gate (artefact)
CICIDS2017, retrospective check (analysis record)
Development / calibration
1.10
1.05
1.00
0.95
0.90
25
50
75
90
95
97
99
99.5
Percentile