FLUKE®
Calibration

Certificate of Calibration
Fluke Calibration
Wuhu Laboratory


Description:	LOOP CALIBRATOR	**Certificate Number:**	3000459028
Manufacturer:	FLUKE CORPORATION	**Date of Calibration:**	08 Jan 2026
Model:	709H	**Date Due:**	
Serial Number:	7130409	**Temperature:**	20 to 26 °C
Status:	AS-LEFT	**Relative Humidity:**	10 to 70 %RH
		Pressure:	95 to 103 kPa
Calibration:	FULL	**Issue Date:**	08 Jan 2026
Procedure:	Fluke 709H:(1 year)CAL/FINAL VER RS-232/M3001 : 1.03		

Customer:

This calibration is traceable to the International System of Units (SI) through recognized national metrology institutes (NIST, PTB, NPL, NIM, NRC, etc.), ratiometric techniques, or natural physical constants. The Quality Management System is certified and is in conformance with !SO 9001 This certificate applies to only the item identified and shall not be reproduced except in full, without the specific written approval by Fluke Corporation.

If measurement uncertainties are provided on the certificate of calibration, they are calculated in accordance with the method described in the ISO Guide to the Expression of Uncertainty in Measurement (GUM). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 % and k=2.

Comments:

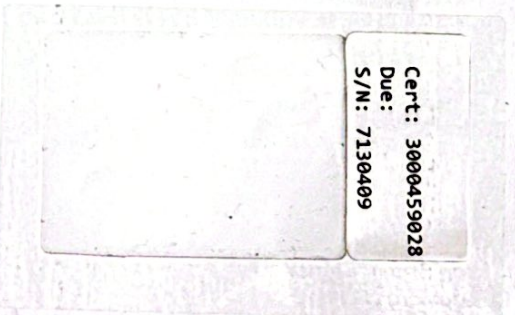

Chen Dandan
Calibration Technician

Scanned with CamScanner

Standards Used

Description	Serial Number	Due-Date
MARTEL ELECTRONICS M3001 MULTIFUNCTION CALIBRATOR	1849213	07-Jul-2026

Quality Manuals

This calibration has been completed in accordance with:

- The Fluke Corporate Quality Manual, Revision 130 and/or
- The Fluke 17025 Quality Manual, Revision 009

Scanned with CamScanner

Applied	Test Result	Error	Specification
mA Source Verification			
4.000 mA	4.0002 mA	0.0002 mA	0.0024 mA
12.000 mA	11.9998 mA	-0.0002 mA	0.0032 mA
20.000 mA	20.0001 mA	0.0001 mA	0.0040 mA
mA Read Verification			
4.0000 mA	4.000 mA	0.0000 mA	0.002 mA
12.0000 mA	11.999 mA	-0.0010 mA	0.003 mA
20.0000 mA	19.999 mA	-0.0010 mA	0.004 mA
V Read Verification			
0.0000 V	0.000 V	0.0000 V	0.002 V
14.0000 V	14.000 V	0.0000 V	0.003 V
28.0000 V	28.000 V	0.0000 V	0.005 V

Scanned with CamScanner