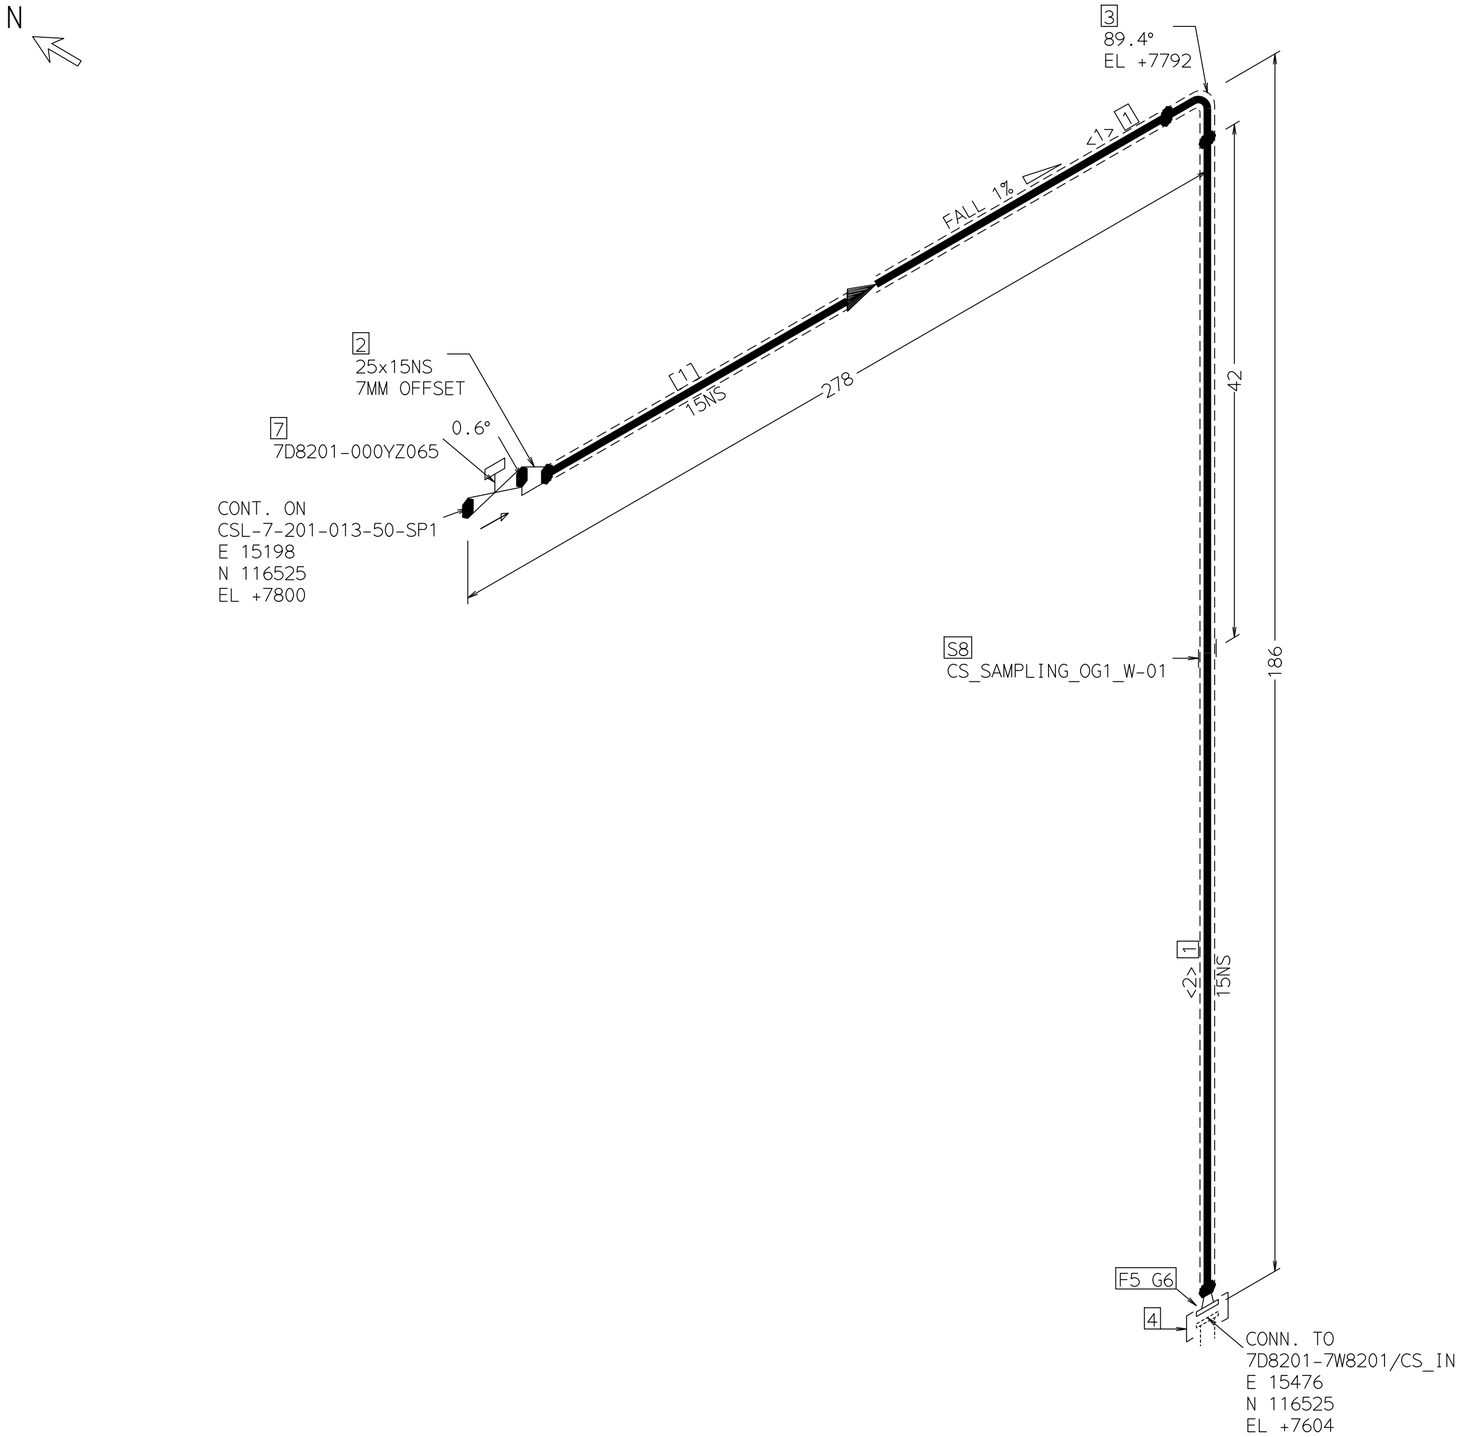

FABRICATION MATERIALS

PT NO	COMPONENT DESCRIPTION	N.S. (MM)	ITEM CODE	QTY
	PIPE			
1	Pipe - seamless or welded - DIN 11866 series B acc.to Pipespec	15	SP1/PPAB6541-PB00_015	0.2M
	FITTINGS			
2	Reducer - design RE (eccentric) - DIN 11865 series B acc.to Pipespec	25 x 15	SP1/EX0B6541-VB00_025-015	1
3	Elbow 90° - type BL-90 - DIN 11865 series B acc.to Pipespec	15	SP1/EB0B6541-PB00_015	1
4	Clamp with anti-tipping device for TC acc.to Pipespec	15	SP1/BKF26001-S000_015	1
	FLANGES			
5	Clamp connection - flat sealing surface - DIN 32676 series B, TC50.5mm acc.to Pipespec	15	SP1/FKF16541-0B41_015	1
	GASKETS			
6	TC seal-DIN 32676 - GYLON 3504 - Gylon 3504	15	SP1/GP089611-0B00_015	1
	INSTRUMENTS			
7	Ball valve - orbital welding ends - pneumatic operated 7D8201-000YZ065	25		1

ERECTION MATERIALS

PT NO	COMPONENT DESCRIPTION	N.S. (MM)	ITEM CODE	QTY
	SUPPORTS			
8	ASSEMBLY GROUP BG15-F80-1/2", DN 15; ARTICLE NO. 110227	15	SIK/BG15-F80-1/2-15	1
	PIPE SPOOLS			
	[1]			

CUT PIPE LENGTH

ITEM CODE	PIECE NO	CUT LENGTH	N.S. (MM)	REMARKS	END PREP.
SP1/PPAB6541-PB00_015	<1>	53	15		BE/BE
SP1/PPAB6541-PB00_015	<2>	95	15		BE/BE

Rev.	Date	Description	Issued	Checked	Released
02	18 Jan 2024	AFC	THPR	DATL	JYEN
01	30 Nov 2023	For review	JYEN	DATL	JUCH

Construction and connection dimensions must be checked on site!
All axis and positions must be checked on site!

peleven®

ThermoFisher SCIENTIFIC

Issued for construction: Date: 18 Jan 2024 Signature:

Pipe class	Insulation	Floor
SP1	H2	1
P&ID-No.	CH06822004-BD-PI-1179	

Project: 5K SUT | Project-No. Peleven | CH06823001

Isometric Number / Pipe name: CSL-7-201-017-25-SP1

Page 1 / 1