

Name:

OD



ID: 103272

Exam Date: 9/11/2023

CZMI

DOB:

Exam Time: 1:46 PM

Gender: Male


Serial Number: 6000-11532

Technician: Operator, Cirrus


Signal Strength: 10/10

## En Face Analysis : Macular Cube 512x128

OD ☒ OS ☐

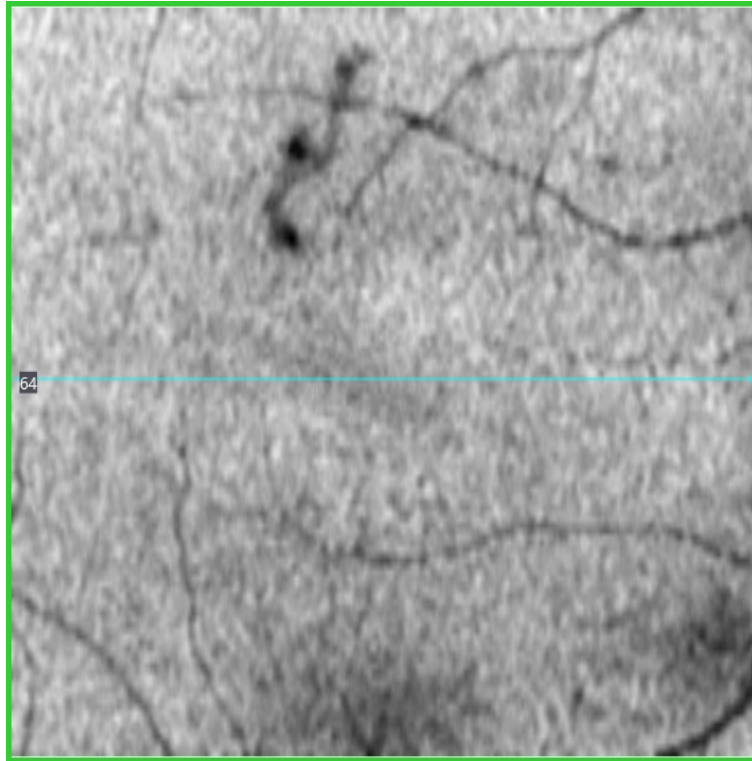


Minimum Intensity: Offset = 10% Range = 90%

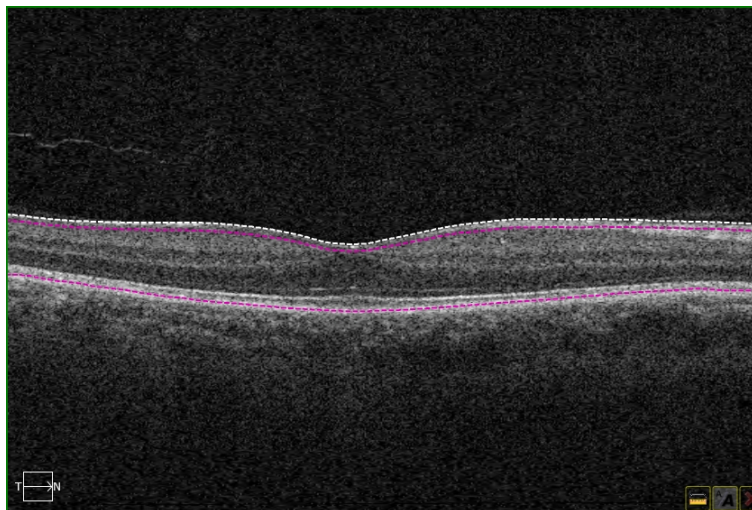


Slice: 64


Thickness Map




OCT Fundus




VRI




Mid-Retina



IS/OS-Ellipsoid




Choroid




Minimum Intensity



Custom - (OCT Fundus)



Custom - (OCT Fundus)



Comments

Doctor's Signature

STORESERV  
SW Ver: 11.5.2.54532  
Copyright 2020  
Carl Zeiss Meditec, Inc  
All Rights Reserved

Page 1 of 1