Importing & Inspecting DICOM Series

Orthanc Web Viewer – Quick Start Guide

Document ID	Version	Date
UG-MED-2026-01	1.0	20/10/2026
Author	**Organization**	**Document Type**
Carolina Couto	Sample SaaS Systems	Public Portfolio Sample

1. Purpose & Scope

This Quick Start Guide provides healthcare professionals and technical teams with standard operational instructions for uploading, querying, and inspecting DICOM datasets within the Orthanc Server environment using the integrated Web Viewer interface.

2. Prerequisites

To successfully launch, upload, and inspect clinical image series, verify the following:

- **Network Access:** Active HTTP connection to the local or cloud Orthanc Server node (default local URL: http://localhost:8042/).
- **Input Datasets:** Valid DICOM files (.dcm format) or compressed study archives (.zip).
- **Browser Compatibility:** HTML5-compliant web browser (Google Chrome, Mozilla Firefox, or Microsoft Edge).

3. Step-by-Step Workflow

Step 1: Accessing the Orthanc Interface & Uploading Studies

1. Open your web browser and navigate to the local Orthanc URL.
2. On the main interface, click the **Upload** button located in the top navigation panel.
3. Drag and drop your target DICOM files into the upload zone or click **Select files** to browse your local directory.
4. Click **Start the upload** and wait for the status indicator to display 100% Complete.

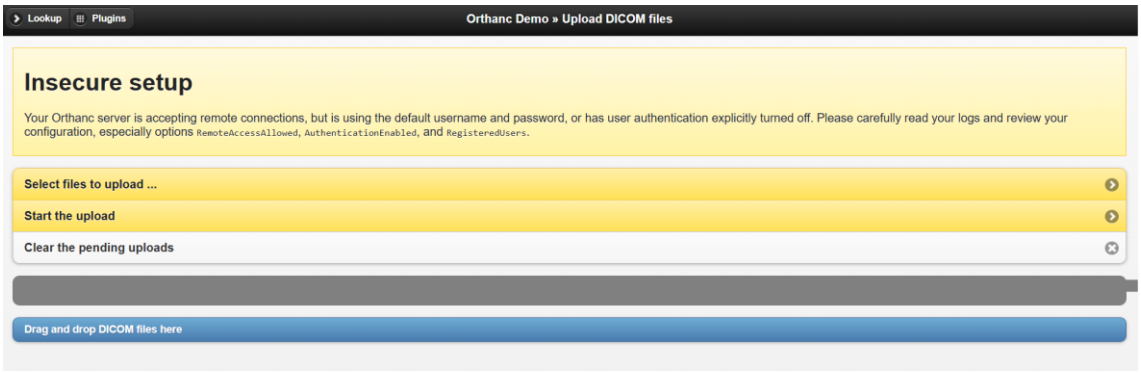


Figure 1 – Orthanc Web Viewer – Upload interface

Step 2: Querying & Inspecting Patient Series

1. Return to the **Patients** or **Studies** tab on the main dashboard.
2. Use the search bar to filter studies by **Patient ID**, **Patient Name**, or **Modality** (e.g., CT, MR, CR).
3. Select the desired study from the search results to open the DICOM Web Viewer.
4. Utilize the viewer toolbar to adjust windowing (W/L presets), zoom, pan, and cycle through image slices.

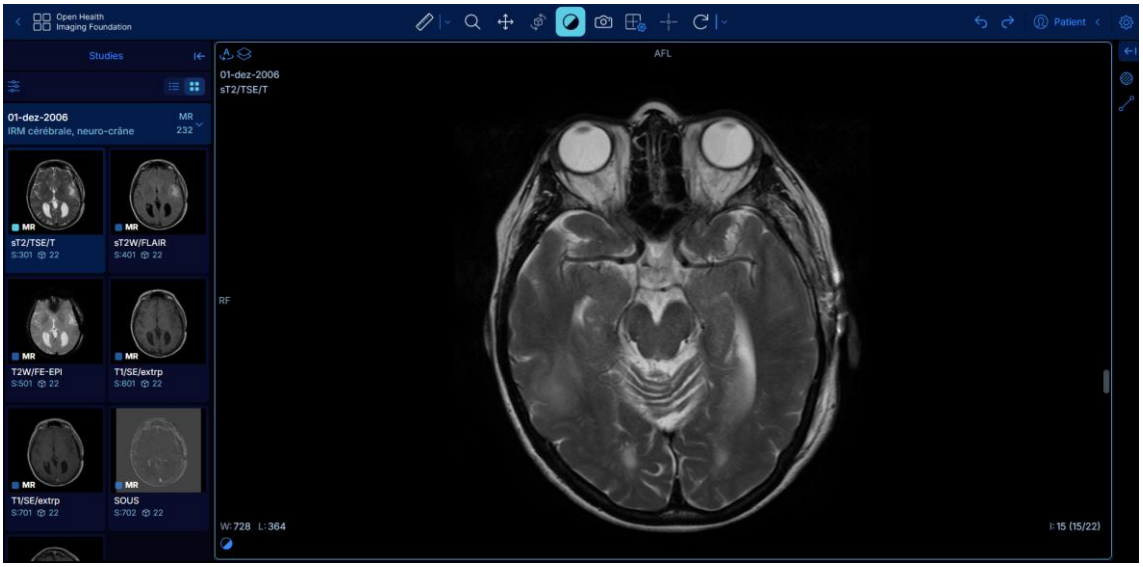


Figure 2 – Integrated DICOM Web Viewer and Tools

4. Viewer Interaction Quick Reference

Action/Function	Mouse/Key Shortcut	Operational Purpose
Slice Navigation	`Mouse scroll`	Navigate sequentially through CT/MR image stack slices.

Window/Level (W/L)	`Left Click + Drag`	Adjust image contrast and brightness dynamically.
Pan Image	`Right Click + Drag`	Reposition the viewing frame across zoomed image regions.
Reset View	`R`	Restore default windowing, zoom level, and orientation.

5. Troubleshooting

- **Error "Bad File Format":** Ensure uploaded files adhere strictly to the DICOM standard (.dcm) and are not corrupted compressed archives.
- **Viewer Fails to Load Slices:** Confirm that your browser has WebGL / Hardware Acceleration enabled and that the web-viewer plugin is enabled in Orthanc's configuration file.

> ⚠️ **IMPORTANT NOTE ON DATA PRIVACY**
> Ensure all uploaded DICOM files comply with regional health data protection policies (e.g., HIPAA / GDPR). De-identification/anonymization must be verified prior to uploading datasets to cloud-hosted or external demonstration nodes.