



Sequence Diagrams

Apply to Skin (UC12)


When the skin bool is set to true the mainWindow starts the timers, when set to false the timers stop and reset.

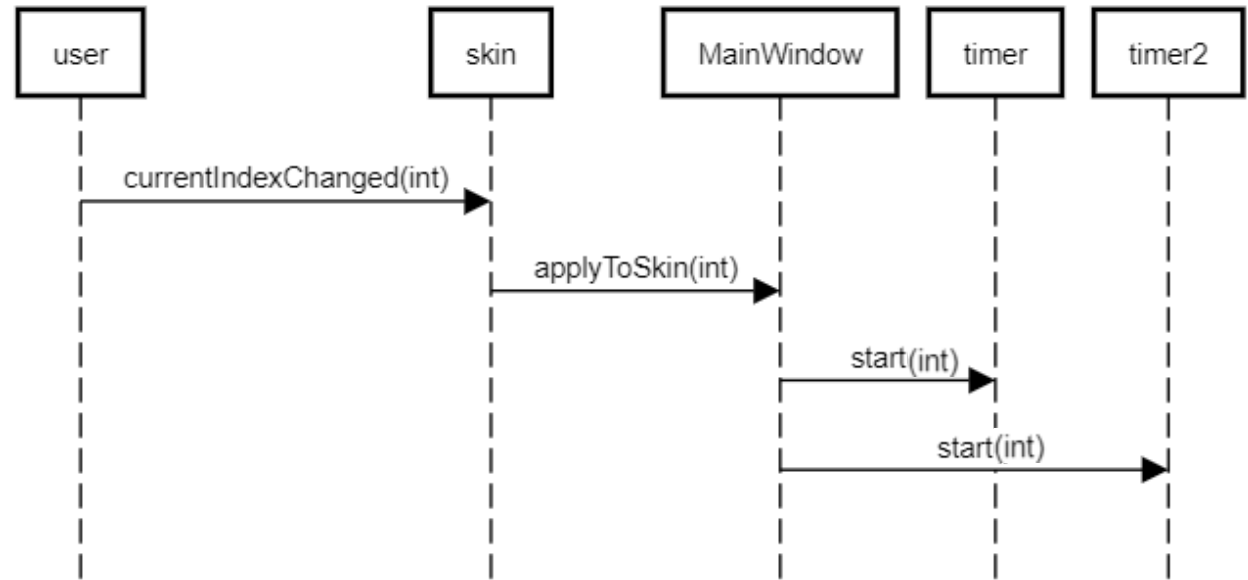

Turn Device On (UC1)

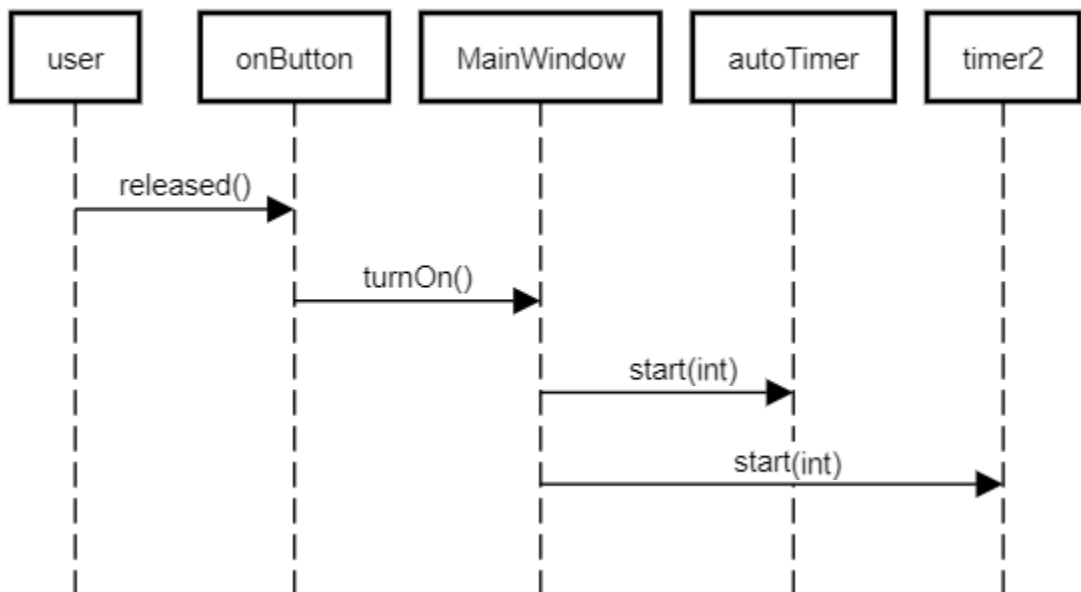


Turn Device Off (UC2)

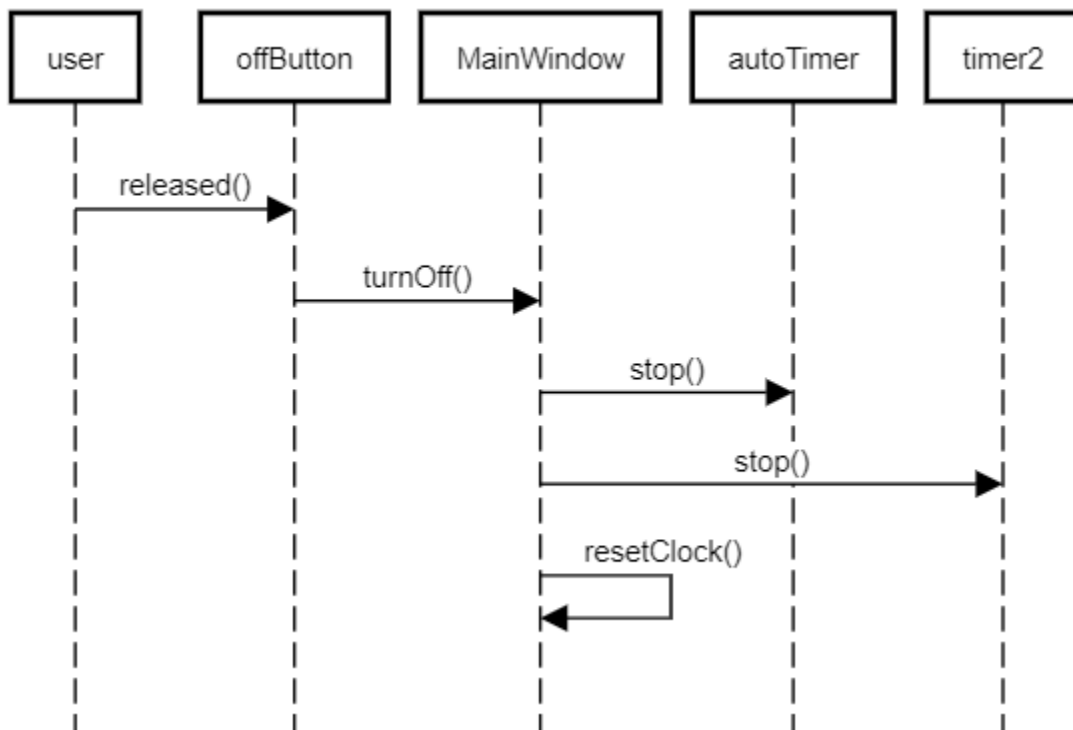

Change Treatment Total Time (UC3)

The time is stored using the clock class.

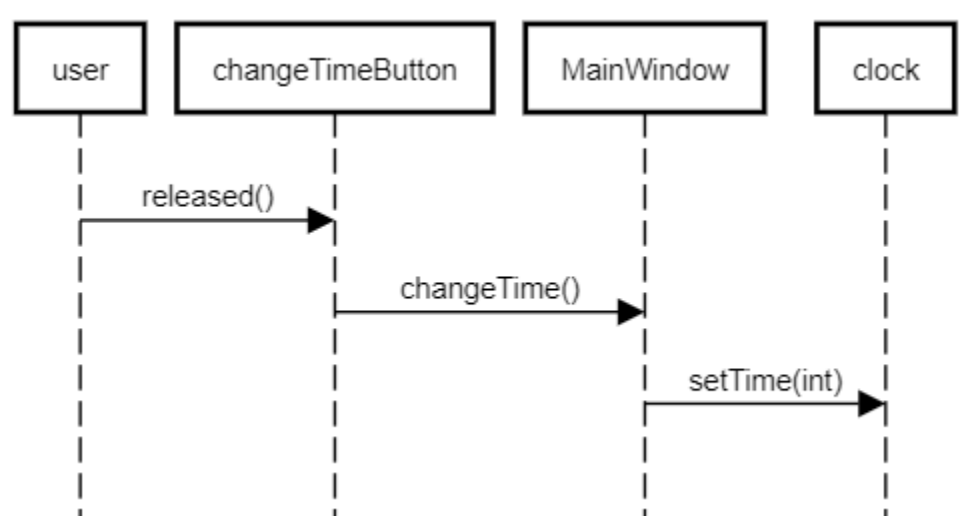

Change Current Intensity (UC6, UC7)

