

# Maintenance Policies for a Multi-Unit System with Adjustable Production Rates

Mark van der Broek

May 31, 2018

## 1 Introduction

Maintenance cost can constitute a large part of the total production costs. For example, Grber (2004) states that maintenance costs can be at much as 30 percent of production costs for power plants, while Bevilacqua and Braglia (2000) give an estimate of between 15 and 70 percent of the total production costs. For this reason, maintenance strategies have been extensively researched in the past decades. Reviews of past research have been published (Horenbeek, Bur, Cattrysse, Pintelon, and Vansteenwegen, 2013; Keizer, Flapper, and Teunter, 2017). Condition-based maintenance (CBM) is an advanced maintenance strategy that is based on performance and/or parameter monitoring and basing subsequent actions on the monitoring.

Condition-based maintenance policies have been proposed for multi-unit systems with economic dependence (Keizer, Teunter, and Veldman, 2016). Keizer, Teunter, Veldman, and Babai (2018) extend this research by including load sharing between units, that is, the deterioration of the functioning units is affected by the number of functioning units, where it is assumed that the load is shared uniformly over all functioning units. In this paper, we consider a system where we relax this assumption and allow the load of all functioning units to depend on the current deterioration level of these units. Setting the load of the functioning units allows to cluster maintenance more effectively. In the rest of the paper, I will use the terminology production instead of load, however observe that production does not assume the production of an item. As I will show in this paper, the effectiveness of setting the production (load) increases with the economic dependence between units.

The coupling of production and maintenance has been the subject of several studies in recent years. Xiang, Cassady, Jin, and Zhang (2014) present an option-based cost model for scheduling a joint production and maintenance policy for a single-period, single-product system. Cheng, Zhou, and Li (2016) study an integrated control strategy of production and maintenance for a machining system which produces a single type of product to meet the constant demand. The authors consider a single-unit system with a preventive maintenance policy.


Offshore wind farms is one of the renewable energy solutions. Since the operation and maintenance costs represent a substantial portion of the total life cycle costs of these offshore wind farms Hau and von Renouard (2003), reliability and condition strategies have drawn increasing interest for decreasing these costs, e.g. Krokoszinski (2003). Existing CBM methods for offshore wind farm systems deal with wind turbines as individual components separately (?). Later maintenance strategies where economic dependence for maintenance actions between wind turbines is taken into account have gained interest (Tian, Jin, Wu, and Ding, 2011). The authors claim a maintenance costs reduction of up to 44.42% compared to maintenance strategies that do not take the economic dependence into account. This reduction is mostly due to the fact that it exploits the large fixed costs from and cluster maintenance actions. One element of the fixed costs component is the cost of sending a maintenance team to the wind farm,, which generally requires expensive vessels.

In this paper, we consider a joint production and maintenance strategy for a multi-unit system. We formulate the system as a Markov Decision Process and analyse the structural properties of the optimal policies. Our model extends the model of Keizer et al. (2018) by allowing the production (load) to be set for all units. The deterioration process of the units is modelled by a discrete-time Markov chain with a known transition probability matrix. The production and maintenance strategy are jointly optimised, while in traditional methods the production is set be uniform for all functioning units.

The remainder of the paper is organised as follows. Section 2 provides the definition and formulation of the system. Section 3 provides a description of the Markov Decision Process used to model the system introduced in Section 2. In Section 4 and 5 the structural properties of the optimal policies of a system with respectively 2 and 3 units is analysed. Conclusions and future research directions are provided in Section 6.

## 2 System formulation

We consider a discrete-time system consisting of  $N$  identical components, which are subject to variable production and economic dependence. We denote the set of units as  $\mathcal{I} = \{1, \dots, n\}$ . The total production that has to be met during every time period is denoted  $\pi$ . Let  $x_i$  denote the deterioration state of unit  $i$ , which deteriorates according to a discrete-time Markov chain with deterioration states  $X = \{0, 1, \dots, L\}$ . State 0 represents the as-good-as-new state,  $L - 1$  denotes the most deteriorated state such that the unit still functions and state  $L$  the failed state. We assume that the production capacity of a unit is not affected by the deterioration state. A schematic overview of the events in one time period is presented in Figure 1.

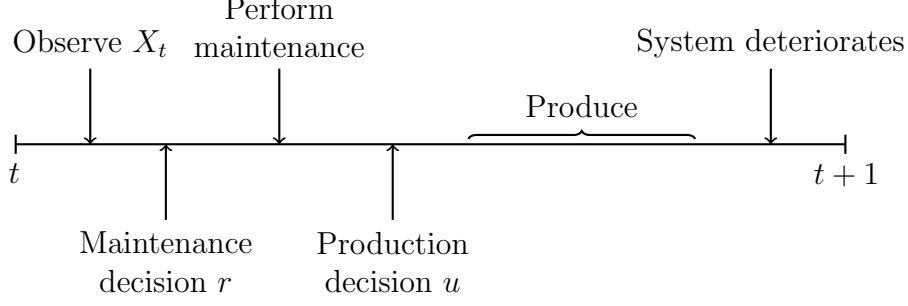

**Figure 1:** Order of events for time epoch  $t$ .

## 2.1 Maintenance and production actions

The deterioration state of each unit is known at the beginning of each time period. This assumption becomes justified for an increasing number of applications, due to better monitoring equipment. Maintenance is assumed to take negligible time and is performed after the deterioration states of each unit is observed. Preventive maintenance is performed at a cost of  $c_{\text{pm}}$  if the unit has not reached the failed state, whereas a corrective maintenance action is performed in the failed state at a cost of  $c_{\text{cm}}$ . Generally, the cost of preventive maintenance is lower than the corrective maintenance action ( $c_{\text{pm}} < c_{\text{cm}}$ ). Performing maintenance on a unit instantaneously brings it back to the as-good-as new state. The economic dependence is included in the form of a fixed cost  $C$  for performing maintenance for a time period. The cost is incurred when at least one unit will be maintained.

After selecting the maintenance action, we also have to set the production rate of each unit. Each unit can produce at most  $m + 1$  different production rates, ranging from 0 to 1 (maximum production). The possible production rates are uniformly distributed over the interval. If a unit is in the failed state, we cannot produce, so the production rate of this unit is set to 0. For all other deteriorating levels, we can select one of the  $m + 1$  production rates.

## 2.2 Deterioration Process

Each unit  $i$  deteriorates according to a gamma process with rate  $\lambda(u_i)$ , which depends on the current production rate of the unit, and scale parameter  $\gamma$ . The rate for a given production rate  $u_i$  is given by


$$\lambda(u_i) = g(u_i)\lambda_{\text{max}},$$

where  $\lambda_{\text{max}}$  is the rate parameter under the maximum production rate, and  $g$  is a non-decreasing function. We assume that  $g(u_i)$  as a function of the production rate  $u_i$  for unit  $i$  is of the following form

$$g(u_i) = \beta + (1 - \beta)u_i^\alpha.$$

We assume that  $0 \leq \beta \leq 1$  and  $\alpha \geq 0$ , since  $g$  should be non-decreasing in  $u_i$ . If the production rate  $u_i$  is zero, then  $g$  has value  $\beta$  i.e.,  $\beta$  determines the deterioration rate if

the unit does not produce. The parameter  $\alpha$  determines the curvature of the function  $g$ . In Figure 2 the function  $g$  is plotted for several settings of  $\alpha$  and  $\beta$ .

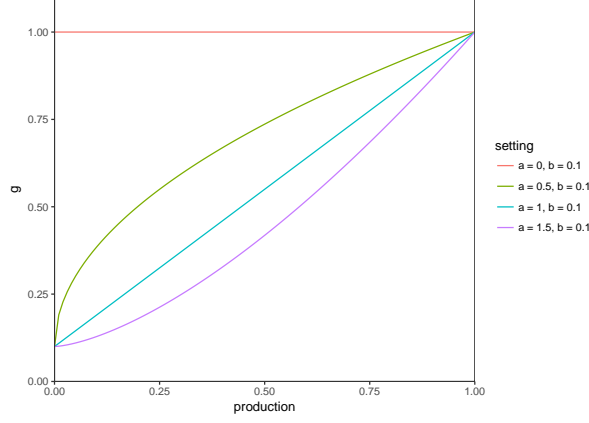

**Figure 2:** Function  $g$  for values  $\alpha = 0, 0.5, 1, 1.5$  and  $\beta = 0.1$ .

The discrete jump probabilities for the gamma process are obtained by discretising the gamma process. One property of the gamma process is that the jump probabilities are independent of the current state. We denote the probability of having a jump of size  $j$  with rate parameter  $a$  and scale parameter  $b$  by  $p(j; a, b)$ . The derivation of the jump probabilities can be found in the manuscript by De Jonge on pages 51-53.

### 3 Markov Decision Process

In this section I provide the Markov Decision Process (MDP) formulation of the system as described in Section 2. The MDP consists of a state space, action space, transition probabilities, expected costs and a performance evaluation.

#### 3.1 State space

We consider a multi-unit system that consists of  $n$  identical units. We denote the set of units as  $\mathcal{I} = \{1, \dots, n\}$ . Each unit deteriorates according to a discrete-time Markov chain with deterioration states  $X = \{0, 1, \dots, L\}$ . State 0 represents the as-good-as-new state and state  $L$  the failed state. The whole state of all units is denoted by

$$x = (x_1, \dots, x_n) \in X^n.$$

#### 3.2 Action space

At the start of each time unit we have to decide on which components to maintain (M) and do nothing (DN). Maintenance can be performed on all units, independent of the

current state, i.e., the action space for the maintenance decision can be defined as

$$R = \{r = (r_1, \dots, r_n) : r_i \in \{\text{DN}, \text{M}\}, \forall i \in \mathcal{I}\}.$$

We define the set of possible production rates for unit  $i$  in state  $x_i$   $U(x_i)$  as follows

$$U(x_i) = \begin{cases} \{0, 1/m, \dots, 1\} & \text{if } x_i \neq L, \\ \{0\} & \text{if } x_i = L. \end{cases}$$

Let  $u = (u_1, \dots, u_n)$  denote the production rate of all units in the system. The total production of the system is restricted to  $\pi$ , i.e.,  $\sum_{i=1}^n u_i = \pi$ . This results in the following action space for the system in state  $x$

$$U(x) = \left\{ u : \sum_{i=1}^n u_i = \pi, u_i \in U(x_i) \forall i \in \mathcal{I} \right\}.$$

Note that the production action space decreases from  $(m+1)^n$  elements to  $\binom{n+\pi-1}{\pi-1}$  by restriction the total production rate to the value  $\pi$ .

### 3.3 Transition probabilities

For a unit  $i$  the probability of having  $q \geq 0$  jumps in the deterioration states for a time epoch under production rate  $u_i$  and scale parameter  $b$  is given by  $p(q; \lambda(u_i), b)$ . The transition probability of unit  $k$  for going from state  $i$  to  $j$  with production rate  $u_i$  and maintenance action DN for any time epoch is defined as

$$P_{u_k, \text{DN}}(i, j) = \begin{cases} p(j-i; \lambda(u_k), b) & \text{if } i \leq j \leq L-1, \\ 0 & \text{if } j < i, \\ 1 - \sum_{l=0}^{L-1-i} p(l; \lambda(u_k), b) & \text{if } i \leq m-1 \text{ and } j = L, \\ 1 & \text{if } i = j = L, \end{cases}$$

and for maintenance action M by

$$P_{u_k, \text{M}}(i, j) = \begin{cases} p(j; \lambda(u_k), b) & \text{if } j \leq L-1, \\ 1 - \sum_{l=0}^{L-1} p(l; \lambda(u_k), b) & \text{if } j = L. \end{cases}$$

Note that for the maintenance action M the probability of going from state  $i$  to  $j$  does not depend on  $i$ , since we assume that the system will go to state 0 immediately after the maintenance action.

The transition probability of a unit in the system is independent of the other units. Therefore, the transition probability that the system goes from state  $x = (x_1, \dots, x_n)$  to state  $\tilde{x} = (\tilde{x}_1, \dots, \tilde{x}_n)$  by selecting production rates  $u$  and maintenance actions  $m$  is given by

$$p(x, \tilde{x} \mid u, m) = \prod_{i=1}^n P_{u_i, m_i}(x_i, \tilde{x}_i),$$

due to independence of the deterioration process of the units.

### 3.4 Expected costs

To define the cost for a time unit, we define a function

$$c(x_i, r_i) = \begin{cases} c_{\text{pm}} & \text{if } r_i = \text{M and } x_i \neq L, \\ c_{\text{cm}} & \text{if } r_i = \text{M and } x_i = L, \\ 0 & \text{elsewhere.} \end{cases}$$

for all states  $x_i \in X$  and maintenance actions  $r_i \in \{\text{DN}, \text{M}\}$  of unit  $i \in \mathcal{I}$ . This means that if unit  $i$  is in the failed state and we decide to perform maintenance, we incur the corrective maintenance costs  $c_{\text{cm}}$ , and if the unit has not failed, then the preventive maintenance costs  $c_{\text{pm}}$  is incurred.

The expected costs for a time unit by selecting maintenance action  $r$  and in state  $x$  is given by

$$\bar{c}(x, r) = \begin{cases} C + \sum_{i=1}^n c(x_i, r_i), & \text{if } r \text{ contains a maintenance action,} \\ 0, & \text{otherwise.} \end{cases}$$

In words, this means that if we do not perform maintenance on any unit for a given time period, we do not incur any costs. However, if we do perform maintenance, we incur the fixed cost  $C$  and some corrective or preventive costs depending on the state of the maintained unit.

### 3.5 Performance criteria

As a performance criterion, we are interested in minimising the long-run average cost per time unit. In this way we can quantify the maintenance costs of a system over the life cycle, and identify the benefits of being able to set the production of each unit.

## 4 Numerical results two-unit system

In this Section we will investigate the key features of the optimal maintenance and production policy for a two-unit system using the MDP as described in Section 3. Similar to Keizer et al. (2018) we select preventive maintenance costs  $c_{\text{pm}} = 5$ , set-up cost  $C = 4$ , and a corrective maintenance cost  $c_{\text{cm}} = 11$ . The rate parameter under the maximum production rate is  $\lambda_{\text{max}} = 0.7$  and the scale parameter  $\gamma = 1$ . The failure level  $L$  and the number of possible production rates are set to 25 and 26, respectively. We vary the total production  $\pi$  with values 20, 30 and 40. For  $\pi = 20$ , one unit can handle all the production and for  $\pi = 40$  we do not have much overcapacity in the system. We set  $\alpha = 0.1$ , such that the deterioration when a unit is not operating is low. We consider three different values for  $\beta$ : 0 (deterioration rate does not depend on production), 1 (deterioration rate depends linearly on production) and 1.5 (deterioration rate is convex in the production).

## 4.1 Benchmark policies

Since the action space of our problem consists of a maintenance action and a production action, we distinguish between a benchmark for the maintenance action and the production action.

In the literature, condition-based maintenance is often implemented in the form of a threshold policy (CITE), or an opportunistic threshold policy (Zhang and Zeng, 2015; Zhou, Xi, and Lee, 2009). In the former policy, if the deterioration level of a unit is at or exceed a threshold level  $T_r$ , we perform a maintenance action. The opportunistic policy adds an additional step to the threshold policy: if a maintenance action is initiated, then all units that have a deterioration state higher or equal to  $T_o$  are also maintained in that time period. The optimal threshold values for  $T_r$  and  $T_o$  are found using a grid search procedure. Due to the economic dependence (fixed cost of maintenance) and the liberty to set the production rate of the components, this policy is probably not optimal. From Figure ?? observe that the optimal maintenance policy is not an opportunistic policy.

**[[Note: I think it is unfair to compare the optimal policy to the standard threshold policy, since this policy is equal or worse than the opportunistic policy. ]]**

Additionally, we need a benchmark policy for the production policy. Inspired by the load sharing formulation in Keizer et al. (2018), we will use the following benchmark for the production policy: For all system states determine the optimal selection of functioning units, where the selected units share the total production  $\pi$  uniformly. The optimal selection is found by minimising the long-run average cost per time unit.

Table (???) presents the

## 4.2 Sensitivity analysis with respect to the maintenance set-up cost

To investigate how the optimal policy and relative effectiveness of the optimal policy compared to the heuristics varies for different levels of economic dependence

### 4.3 Sensitivity analysis with respect to variation in the deterioration process

## 5 Numerical results three-unit system

## 6 Conclusion

Directions for future research in the direction of joint production and maintenance policies for multi-unit systems could be: 1) include dependence between the production capacity of units and its deterioration state, 2) include lead time for planning maintenance and 3) model dependence between the deterioration process of all units due to external shocks. The first extension could be realistic in some applications where the production of a unit is affected by the deterioration of that unit, e.g., semiconductor manufacturing (Kazaz and Sloan, 2013). The second direction is relevant for systems that have a high frequency of maintenance actions relative to the life cycle of the system. The last extension could be relevant when units are affected by, for example, weather conditions. It is realistic to assume that the deterioration of identical units is impacted in a similar way due to bad weather.

## References

- M. Bevilacqua and M. Braglia, “The analytic hierarchy process applied to maintenance strategy selection,” *Reliability Engineering System Safety*, vol. 70, no. 1, pp. 71 – 83, 2000. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0951832000000478>
- G. Q. Cheng, B. H. Zhou, and L. Li, “Joint optimisation of production rate and preventive maintenance in machining systems,” *International Journal of Production Research*, vol. 54, no. 21, pp. 6378–6394, 2016. [Online]. Available: <http://doi.org/10.1080/00207543.2016.1174343>
- U. Grber, “Advanced maintenance strategies for power plant operators?introducing inter-plant life cycle management,” *International Journal of Pressure Vessels and Piping*, vol. 81, no. 10, pp. 861 – 865, 2004, 29th MPA Seminar in the series Safety and Reliability of Pressure Components - Stuttgart, October 9th and 10th, 2003. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0308016104001449>
- E. Hau and H. von Renouard, *Wind turbines: fundamentals, technologies, application, economics*. Springer, 2003.
- A. V. Horenbeek, J. Bur, D. Cattrysse, L. Pintelon, and P. Vansteenwegen, “Joint maintenance and inventory optimization systems: A review,” *International Journal of Production Economics*, vol. 143, no. 2, pp. 499 – 508, 2013, focusing on Inventories: Research and Applications. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0925527312001466>



- B. Kazaz and T. W. Sloan, “The impact of process deterioration on production and maintenance policies,” *European Journal of Operational Research*, vol. 227, no. 1, pp. 88–100, 2013.
- M. C. O. Keizer, R. H. Teunter, and J. Veldman, “Clustering condition-based maintenance for systems with redundancy and economic dependencies,” *European Journal of Operational Research*, vol. 251, no. 2, pp. 531 – 540, 2016. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0377221715010218>
- M. C. O. Keizer, S. D. P. Flapper, and R. H. Teunter, “Condition-based maintenance policies for systems with multiple dependent components: A review,” *European Journal of Operational Research*, vol. 261, no. 2, pp. 405 – 420, 2017. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0377221717301881>
- M. C. O. Keizer, R. H. Teunter, J. Veldman, and M. Z. Babai, “Condition-based maintenance for systems with economic dependence and load sharing,” *International Journal of Production Economics*, vol. 195, pp. 319 – 327, 2018. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0925527317303456>
- H.-J. Krokoszinski, “Efficiency and effectiveness of wind farmskeys to cost optimized operation and maintenance,” *Renewable Energy*, vol. 28, no. 14, pp. 2165–2178, 2003.
- Z. Tian, T. Jin, B. Wu, and F. Ding, “Condition based maintenance optimization for wind power generation systems under continuous monitoring,” *Renewable Energy*, vol. 36, no. 5, pp. 1502–1509, 2011.
- Y. Xiang, C. R. Cassady, T. Jin, and C. W. Zhang, “Joint production and maintenance planning with machine deterioration and random yield,” *International Journal of Production Research*, vol. 52, no. 6, pp. 1644–1657, 2014. [Online]. Available: <https://doi.org/10.1080/00207543.2013.843037>
- X. Zhang and J. Zeng, “A general modeling method for opportunistic maintenance modeling of multi-unit systems,” *Reliability Engineering System Safety*, vol. 140, pp. 176 – 190, 2015. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0951832015000964>
- X. Zhou, L. Xi, and J. Lee, “Opportunistic preventive maintenance scheduling for a multi-unit series system based on dynamic programming,” *International Journal of Production Economics*, vol. 118, no. 2, pp. 361 – 366, 2009. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0925527308003472>

## A Appendix

### A.1 Discretising the gamma process

See Maintenance planning and optimisation literature of Bram de Jonge.