Table of Contents

iMotions Lab > Remote Data Collection (RDC) > Additional RDC Articles

RDC Settings and Stimuli Behavior 2

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

RDC Settings and Stimuli Behavior


Introduction

Similar to iMotions Desktop, there are different features and options that you can set at the study-level and also at the stimulus-level. Some RDC behavior will need to be set in the iMotions desktop software prior to uploading the study to the cloud for data collection. However, most RDC behavior and settings can be accessed using the online experimenter dashboard.

Settings in the Desktop Software

Sensors

You must set the sensor information in the iMotions dekstop software when you are creating the study. You cannot change this once the study has been uploaded to the cloud for data collection.

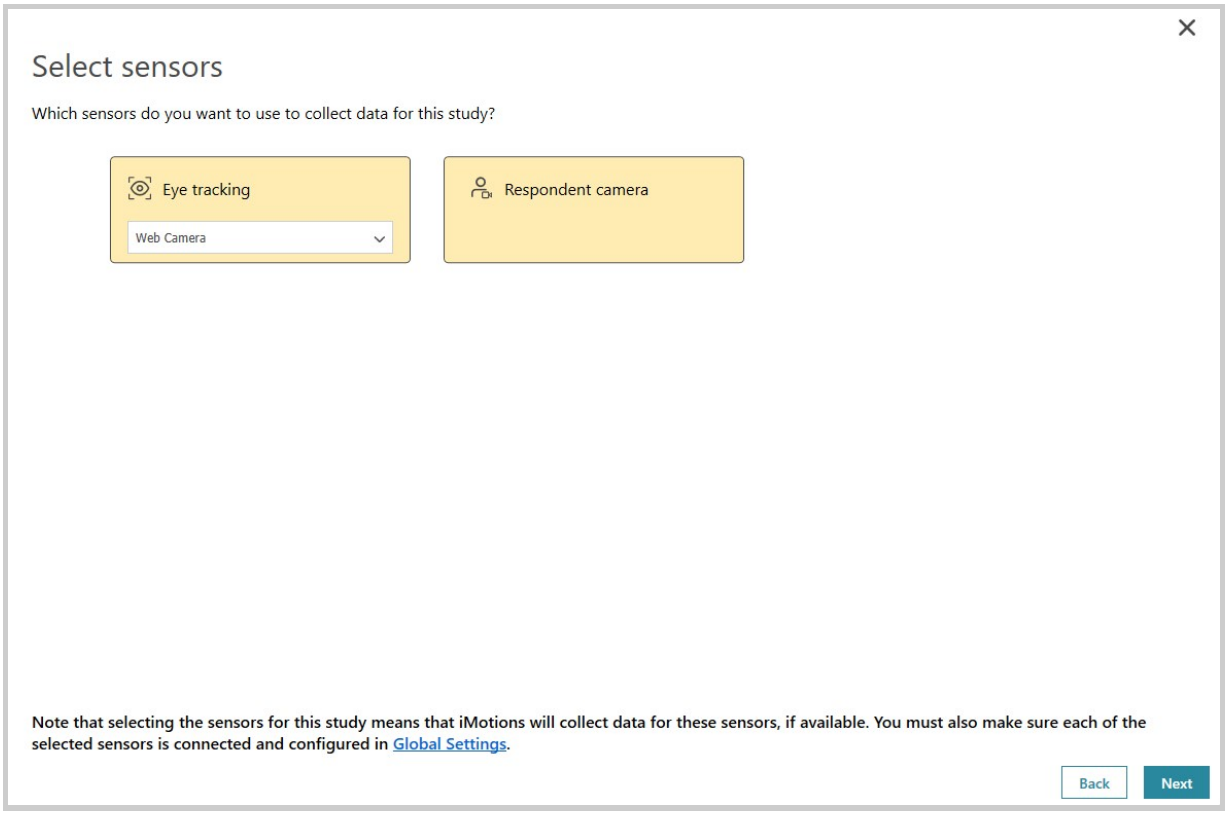

Confidential © 2023 Redistribution is not permitted without written permission from iMotions


1. For webcam-based eye tracking, you can select *Web Camera* as the eye tracking sensor. Note: Web Camera is an option only available in iMotions build 8.2.5 or newer. For older builds of iMotions 8.2, you can use *Mouse Simulator* to trigger the webcam eye-tracking algorithms.
2. A respondent camera is necessary. (Post-processing tools such as Facial expressions and Voice analysis can be done locally if you have the respondent's video recording if you have access)

Stimulus ordering

(In iMotions 10 we reccomend using the new study builder tool to control the flow the stimuli shown during the study. See this article on how to use the study builder. This will give a better overview of the study, We still allow you to set properties individually below on the individual properties screens)

For the online study, you can have stimuli presented in either *fixed* or *randomized* order. When creating your study in the iMotions desktop software, you can simply set up your study as normal and organize your stimuli ordering in Stimuli Ribbon.

To lock a stimulus position in the study flow, remember to check the box as seen below.

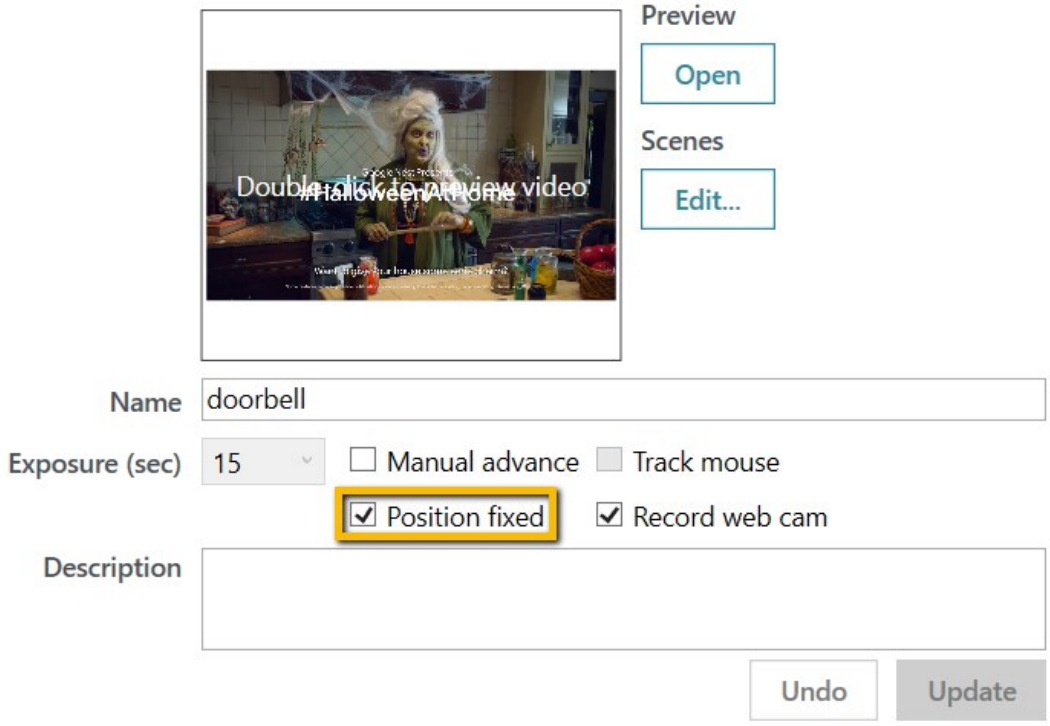


Confidential © 2023 Redistribution is not permitted without written permission from iMotions

Important: In order to present videos, images, or even websites in a randomized manner, you must have *at least* one stimulus that is in a fixed position, for example, your first stimulus can be an instruction slide with fixed position.

(Advanced feature) If you are using a test plan to create your study, you can create pseudo-randomized stimuli orderings for each participant. For more information on setting up a study using a test plan, please refer to RDC Using Test Plans.

Stimulus exposure time limit


For images and website stimuli (including Qualtrics surveys), you must set the exposure time (i.e., maximum duration allowed), in the iMotions desktop software. You cannot change the exposure time limit using the online dashboard once the study has been uploaded to the cloud for data collection!

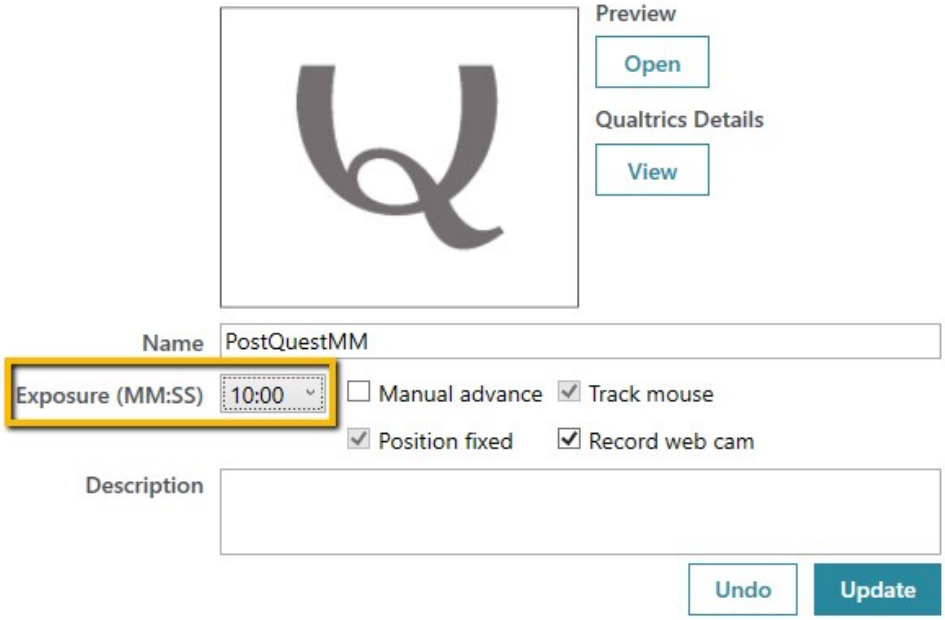

Stimulus advancement

When creating a stimulus, you can set it to *manually* advance or *automatically* advance by leaving it unchecked. Either way, the stimulus will advance after hitting the exposure time limit.

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

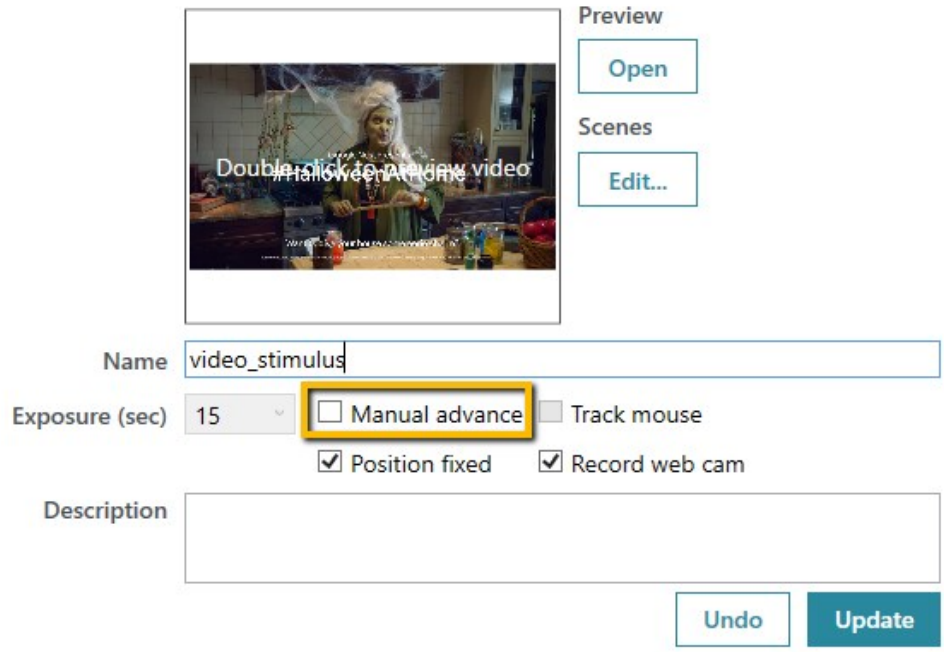


Analysis

When post-processing facial expression analysis data, it is particularly important to ensure that all stimuli are selected when initiating post-processing. All stimuli are selected by default - if any are deselected prior to processing, then the processing will not occur.


Settings in the Online Experimenter Dashboard

When you are using the online experimenter dashboard, you can access a variety of settings by clicking on the *Details* button.

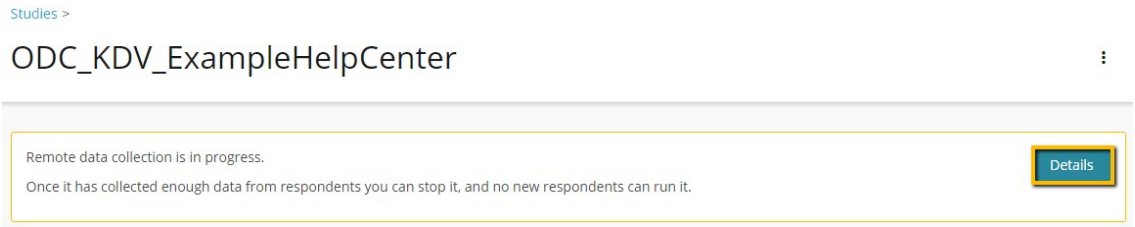

Once you have hit *Details*, you will see the available settings shown below. NOTE: If you have already begun data collection, please select *Stop data collection* in order to see the setting options.

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

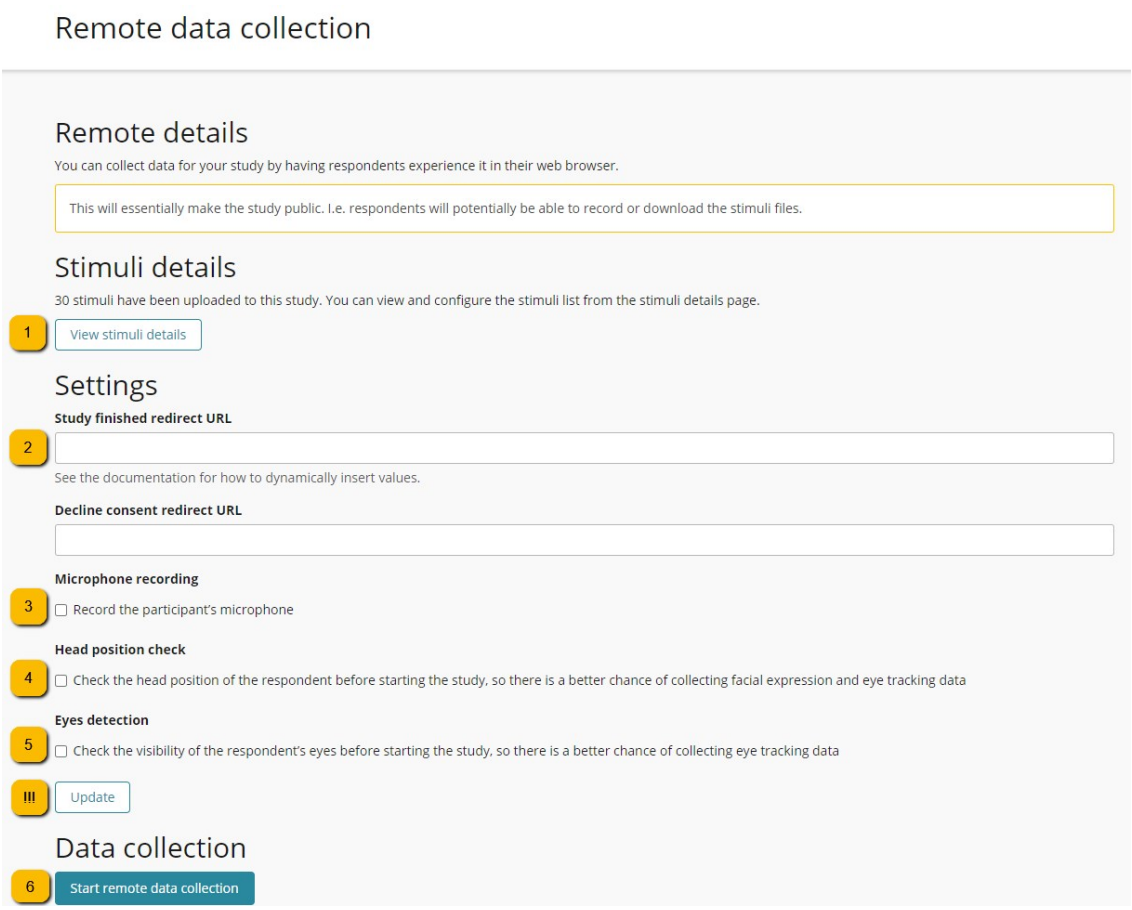

1. View stimuli details. This provides you with the option to change between manual or auto advance for any given stimulus (see below). In addition, you can test for website compatibility with iFrame embedding in this section of the settings, as well. For more information about website behavior and settings, see RDC Testing With Websites .
2. Study finished redirect URL. Participants will automatically be redirected to this URL (within the same window) after the study has completed saving and uploading to the server.
3. Microphone recording. This activates the ability to record the participant's audio (as well as their video) during data collection.
4. Head position check. This turns on (or off) the initial feedback to participants whether they are positioned correctly within their webcam recording (without face occlusion) and whether sufficient light has been identified..
5. Eye detection. This option is automatically turned on if you have opted in for webcam-based eye tracking. Similar to step (4) above, this provides an initial feedback to participants whether their eyes are captured correctly within the video frame without any occlusions.
6. Start remote data collection. Start your study! This generates a study link for you to distribute.

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

(!!!) NOTE: If you have activated (or deactivated) any of the settings above, you must press *Update* prior to pressing *Start remote data collection* in order for the changes to be correctly applied.

Stimulus advancement


In addition to setting stimulus advancement behavior in the desktop software, you can change this setting anytime using your online experimenter dashboard.

1. On the online dashboard, select your study then select *Details* to open more options.


2. Go to *View stimuli details*

NOTE: If you have already begun data collection, please select *Stop data collection* in order to see the *View stimuli details* button.

3. Select the three dots next to each web stimulus to set opening behavior.

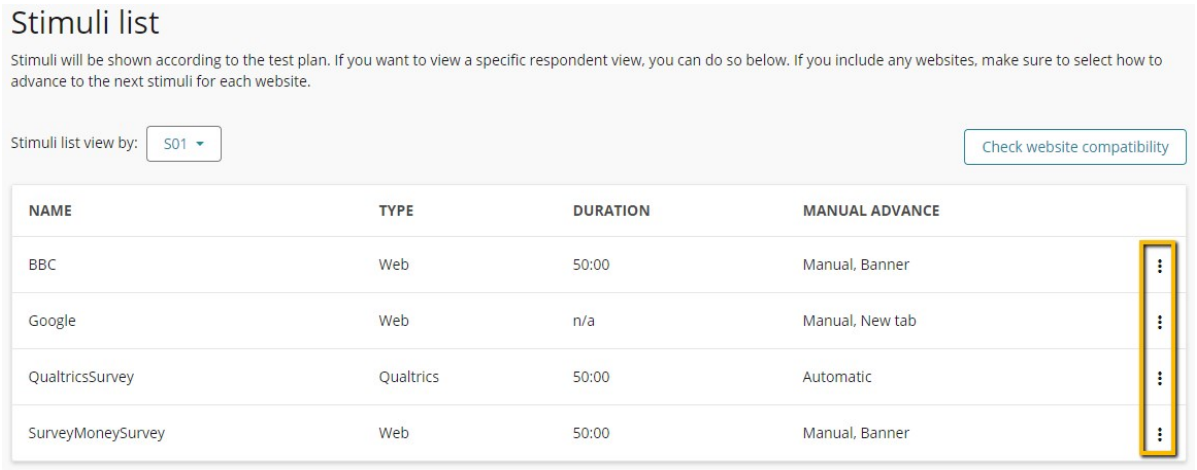

4. A new popup will appear where you can select "Manual advance" or "Automatic advance".

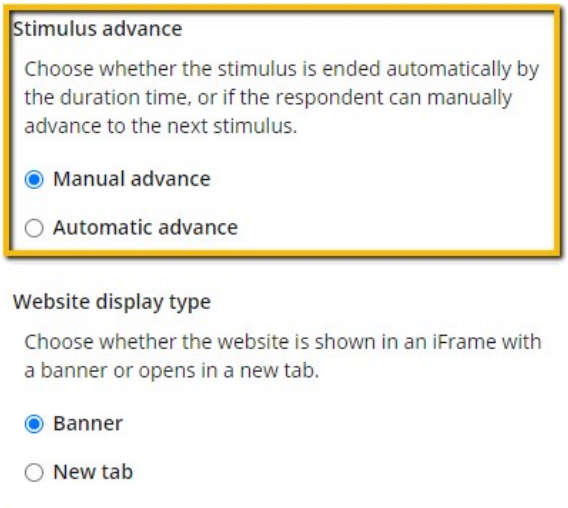

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

Powered by Document360

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

Confidential © 2023 Redistribution is not permitted without written permission from iMotions