Table of Contents

iMotions Lab > iMotions Exports > Additional Export Information

Exports: Open iMotions Sensor Data in Excel 2

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

Exports: Open iMotions Sensor Data in Excel

In the following article, you can see how you can change Excel settings, to default read files, as either Comma or Tab separation.

It will also be shown how Excel can detect what the individual file should be read as.

If you have ever opened a Sensor data export file, and it looked like the image below. Then you should read through this article

Confidential © 2023 Redistribution is not permitted without written permission from iMotions



	A	B	C	D	E	F	G	H	I	J	K	L	M
1	#INFO,,,,,,,,,,,,,,,,,,,,												
2	#Study name,Study 19-08-19 14h40m,,,,,,,,,,,,,,,,,,,,												
3	#Respondent Name,Anonymous 19-08-19 14h47m,Id: f12d9f5e-1e44-4376-a410-280fff83a976,,,,,,,,,,,,,,,,,,,,												
4	#Respondent Age,0,,,,,,,,,,,,,,,,,,,,												
5	#Respondent Gender,MALE,,,,,,,,,,,,,,,,,,,,												
6	#Respondent Group,Default,,,,,,,,,,,,,,,,,,,,												
7	#iMotions version,8.0.16373.3,,,,,,,,,,,,,,,,,,,,												
8	#Current culture,da-DK dansk (Danmark),File encoding: System.Text.UTF8Encoding,Date format: dd-MM-yyyy,,,,,,,,,,,,,,,,,,												
9	#Recording time,Date: 19-08-2019,Time: 14:47:57.198 +02:00,Unix time: 1566218877,,,,,,,,,,,,,,,,,,												
10	#Export time,Date: 02-09-2019,Time: 13:29:57.231 +02:00,,,,,,,,,,,,,,,,,,												
11	#Sensor info,Eyetracker Mouse Simulator, Latency: 0 milliseconds,,,,,,,,,,,,,,,,,,												
12	#,,,,,,,,,,,,,,,,,,,,												
13	#METADATA,,,,,,,,,,,,,,,,,,,,												
14	#Device,iMotions,SlideEvents (iMotions),SlideEvents (iMotions),SlideEvents (iMotions),SlideEvents (iMotions),SlideEvents (iMotions												
15	#Category,Timestamp,Slideshow,Slideshow,Slideshow,Slideshow,Slideshow,Event Source,,ETGaze,ETGaze,ETGaze,ETGaze,ETGaze,ET(												
16	#Description,iMotions synchronization timestamp. Relative to data recording start,Slide & Media events: Start/Stop,Type of stimulus,S												
17	#Unit,Millisecond,,,Millisecond,,,,,Pixel,Pixel,Pixel,Pixel,Millimeter,Millimeter,Millisecond,Centimeter,Centimeter,Relative position												
18	#DataType,Double,String,String,Double,String,String,Boolean,Double,Double,Double,Double,Double,Double,Double,Double,Double,												
19	#,,,,,,,,,,,,,,,,,,,,												
20	#DATA,,,,,,,,,,,,,,,,,,,,												
21	Row,Timestamp,SlideEvent,StimType,Duration,CollectionPhase,SourceStimuliName,EventSource,ET_MediaTime,ET_GazeLeftx,ET_Ga												
22	1,509.4197,StartSlide,TestImage,300000,StimuliDisplay,AdobeStock_58064010,1,,,,,,,,,,,,,,												
23	2,513.4091,,,,,,,,1845,720,1845,720,5,5,500,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
24	3,518.3957,StartMedia,TestImage,300000,StimuliDisplay,AdobeStock_58064010,1,,,,,,,,,,,,,,												
25	4,533.3949,,,,,,,,1845,720,1845,720,5,5,520,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
26	5,553.3338,,,,,,,,1845,720,1845,720,5,5,540,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
27	6,573.2806,,,,,,,,1845,720,1845,720,5,5,560,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
28	7,593.196,,,,,,,,1845,720,1845,720,5,5,580,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
29	8,613.1914,,,,,,,,1845,720,1845,720,5,5,600,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
30	9,633.2722,,,,,,,,1845,720,1845,720,5,5,620,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
31	10,653.0348,,,,,,,,1845,720,1845,720,5,5,640,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
32	11,673.1458,,,,,,,,1845,720,1845,720,5,5,660,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
33	12,692.962,,,,,,,,1845,720,1845,720,5,5,680,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
34	13,713.8731,,,,,,,,1845,720,1845,720,5,5,701,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
35	14,733.8237,,,,,,,,1845,720,1845,720,5,5,721,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
36	15,753.0886,,,,,,,,1845,720,1845,720,5,5,740,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
37	16,773.0888,,,,,,,,1845,720,1845,720,5,5,760,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
38	17,793.0586,,,,,,,,1845,720,1845,720,5,5,780,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
39	18,813.7547,,,,,,,,1845,720,1845,720,5,5,801,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
40	19,833.8813,,,,,,,,1845,720,1845,720,5,5,821,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
41	20,853.8215,,,,,,,,1845,720,1845,720,5,5,841,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
42	21,873.4502,,,,,,,,1845,720,1845,720,5,5,860,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
43	22,893.7163,,,,,,,,1845,720,1845,720,5,5,881,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
44	23,913.6489,,,,,,,,1845,720,1845,720,5,5,901,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
45	24,933.4536,,,,,,,,1845,720,1845,720,5,5,920,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
46	25,953.3976,,,,,,,,1845,720,1845,720,5,5,940,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
47	26,973.2918,,,,,,,,1845,720,1845,720,5,5,960,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
48	27,993.4546,,,,,,,,1845,720,1845,720,5,5,980,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
49	28,1013.0927,,,,,,,,1845,720,1845,720,5,5,1000,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
50	29,1033.3385,,,,,,,,1845,720,1845,720,5,5,1020,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
51	30,1053.3345,,,,,,,,1845,720,1845,720,5,5,1040,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
52	31,1073.2354,,,,,,,,1845,720,1845,720,5,5,1060,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
53	32,1093.2164,,,,,,,,1845,720,1845,720,5,5,1080,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
54	33,1113.8075,,,,,,,,1845,720,1845,720,5,5,1101,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
55	34,1133.75,,,,,,,,1845,720,1845,720,5,5,1121,650,650,0.56366276741027832,0.5,0.36366277933120728,0.5,1												
56	35,1153.6962,,,,,,,,1841,713,1841,713,5,5,1141,650,650,0.56482559442520142,0.49513888359069824,0.36482557654380798,0.495138883590												

003_Anonymous 19-08-19 14h47m


The way you change how excel reads the specific file, is by clicking

1. Go to the Data-tab and select From Text/CSV.
2. Select the file you want to import from your file system and press Get Data.
3. Excel should detect which parameter has by default be used, and will

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

suggest these configurations.

4. Click Load.

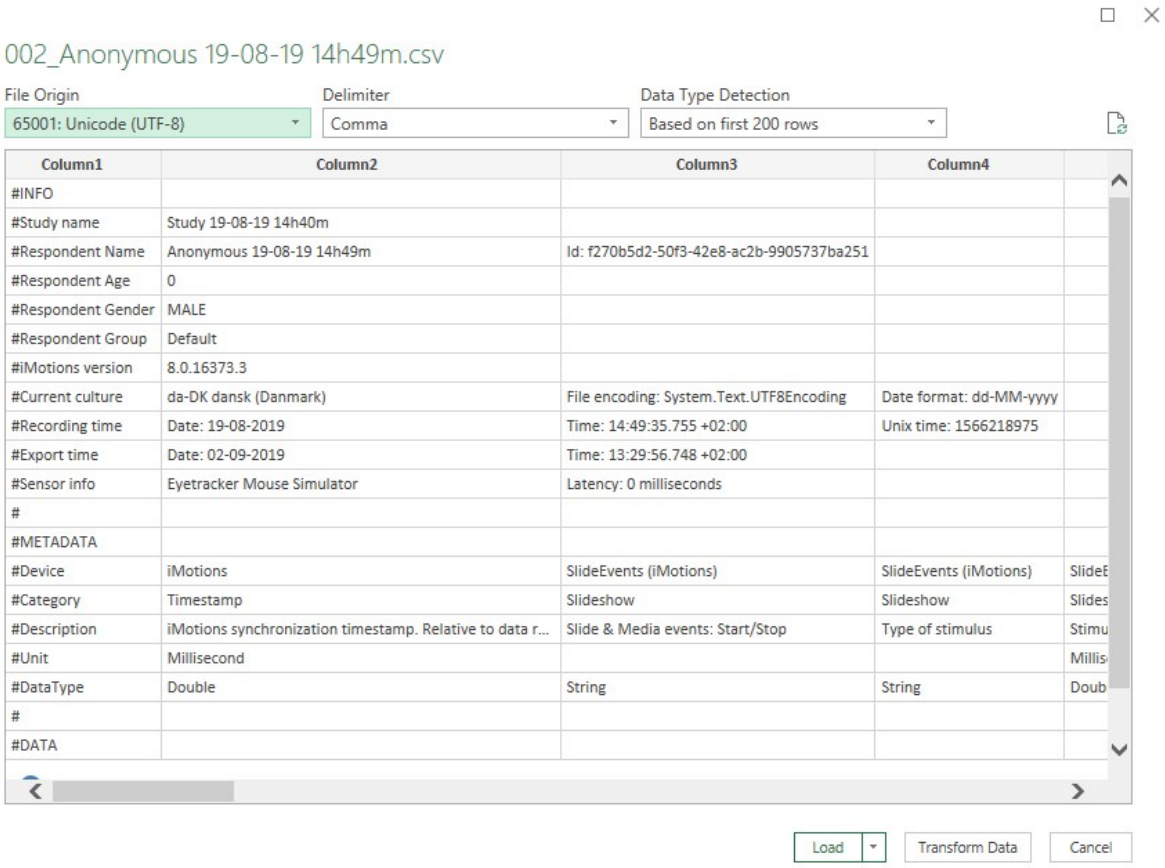


Column1	Column2	Column3	Column4	
#INFO				
#Study name	Study 19-08-19 14h40m			
#Respondent Name	Anonymous 19-08-19 14h49m	Id: f270b5d2-50f3-42e8-ac2b-9905737ba251		
#Respondent Age	0			
#Respondent Gender	MALE			
#Respondent Group	Default			
#iMotions version	8.0.16373.3			
#Current culture	da-DK dansk (Danmark)	File encoding: System.Text.UTF8Encoding	Date format: dd-MM-yyyy	
#Recording time	Date: 19-08-2019	Time: 14:49:35.755 +02:00	Unix time: 1566218975	
#Export time	Date: 02-09-2019	Time: 13:29:56.748 +02:00		
#Sensor info	Eyetracker Mouse Simulator	Latency: 0 milliseconds		
#				
#METADATA				
#Device	iMotions	SlideEvents (iMotions)	SlideEvents (iMotions)	SlideE
#Category	Timestamp	Slideshow	Slideshow	Slides
#Description	iMotions synchronization timestamp. Relative to data r...	Slide & Media events: Start/Stop	Type of stimulus	Stimu
#Unit	Millisecond			Millis
#DataType	Double	String	String	Doub
#				
#DATA				

Note, that depending on which export you use, the settings will not always be the same, but excel is smart enough to suggest the "correct" format.

If you find yourself always doing this, therefore, you might aswell just have it read the file in this manner by default, then go to the following menu

1. In Microsoft Windows, click the Start button, and then click Control Panel.
2. Open the dialog box for changing Regional and Language settings.
3. Click Additional settings...
4. Type a new separator in the List separator box.
5. Click OK twice.

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

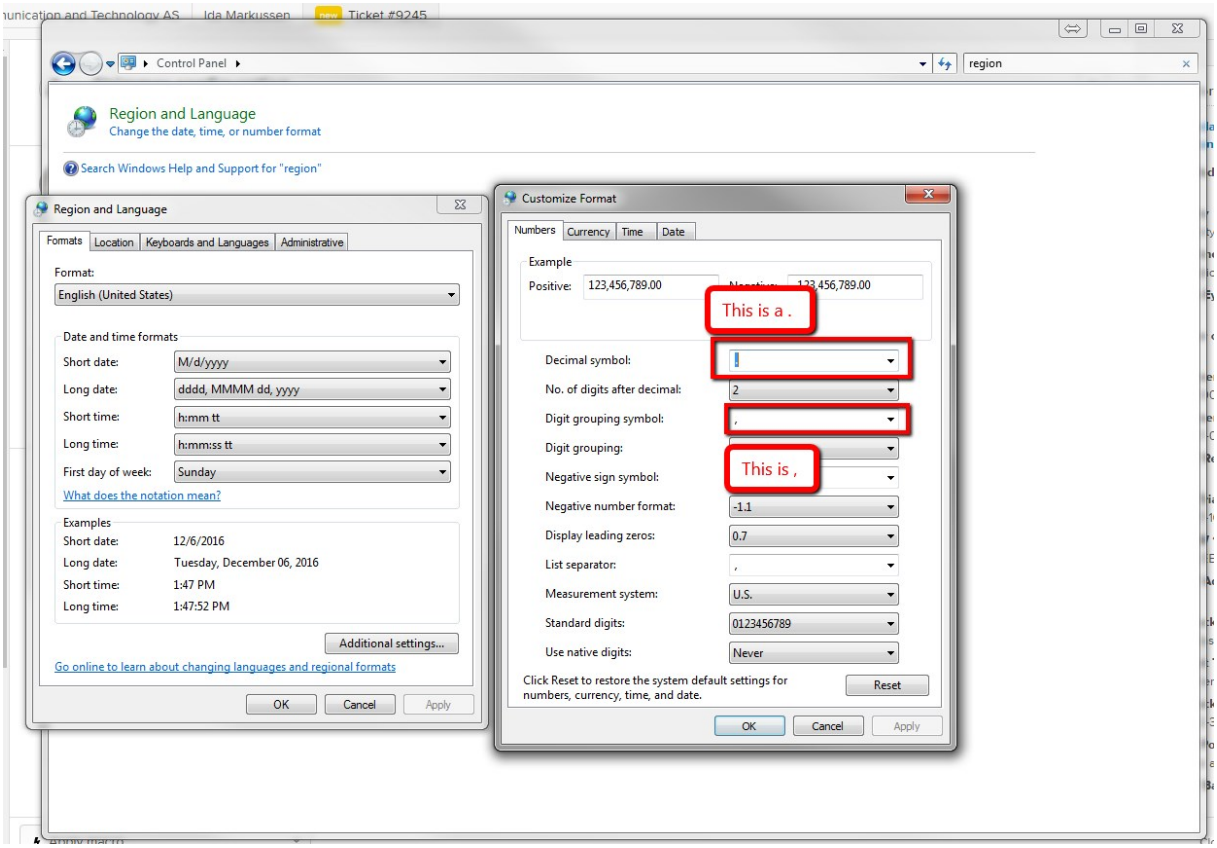

Powered by Document360

Confidential © 2023 Redistribution is not permitted without written permission from iMotions

Confidential © 2023 Redistribution is not permitted without written permission from iMotions