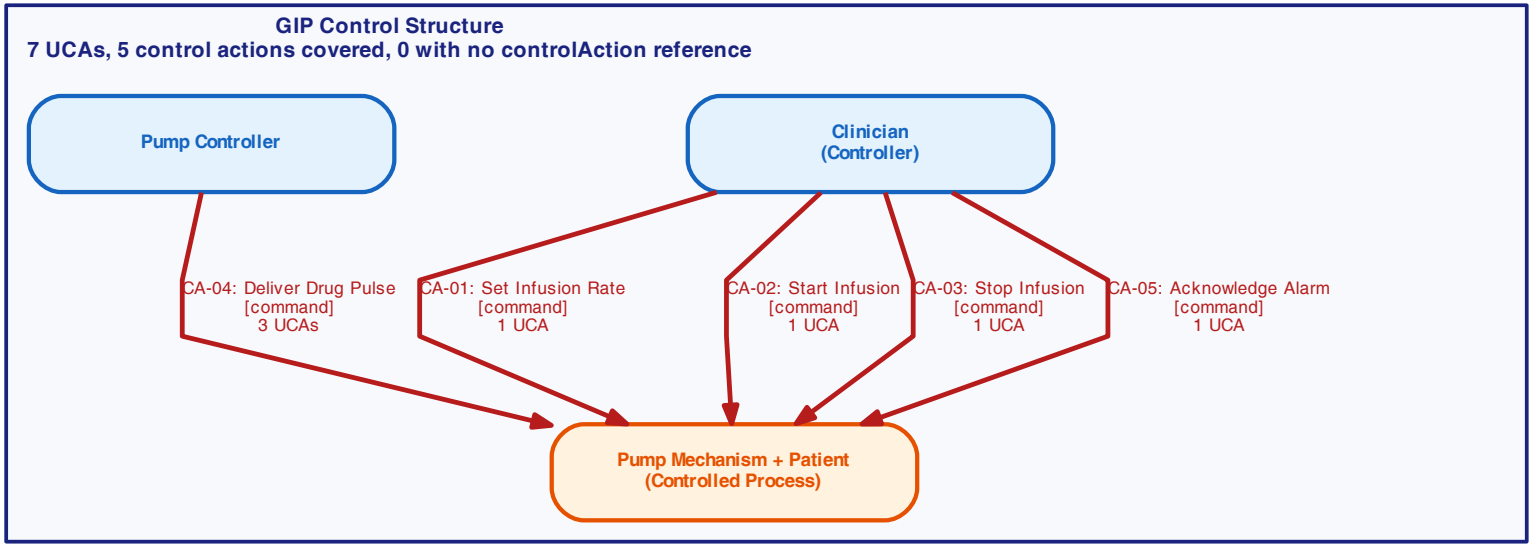
GIP Control Structure
7 UCAs, 5 control actions covered, 0 with no controlAction reference
Pump Controller
Clinician
(Controller)
CA-04: Deliver Drug Pulse
[command]
3 UCAs
CA-01: Set Infusion Rate
[command]
1 UCA
CA-02: Start Infusion
[command]
1 UCA
CA-03: Stop Infusion
[command]
1 UCA
CA-05: Acknowledge Alarm
[command]
1 UCA
Pump Mechanism + Patient
(Controlled Process)