
## flora2o - Pump Off; Active



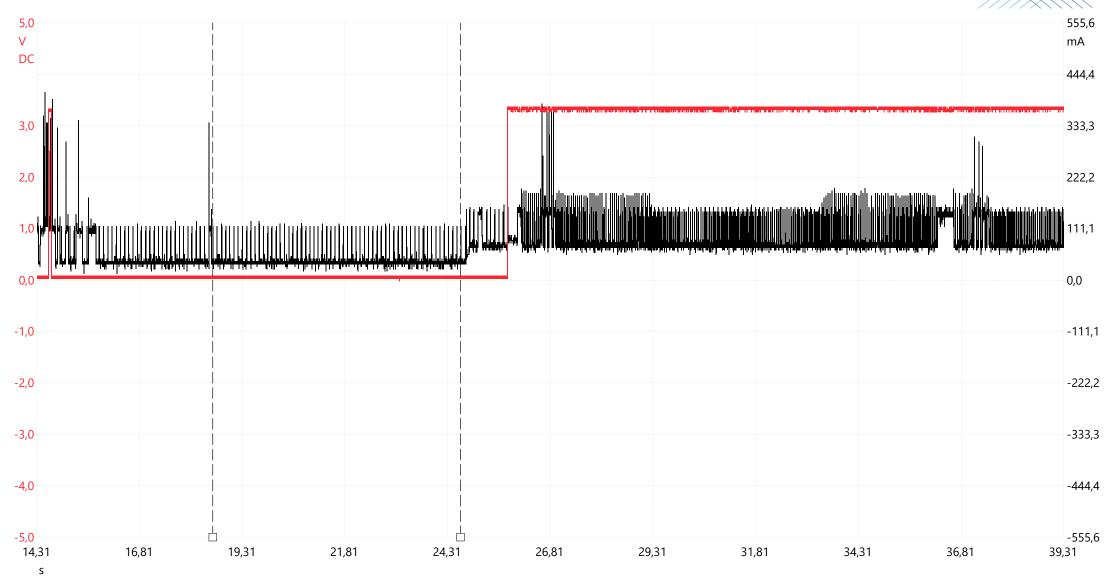

13.06.2021 19:30:44

 Channel
 Name
 Span
 Value
 Min
 Max
 Average
 σ

 -A/0,9
 DC Average
 Between rulers
 42,51 mA
 42,51 mA
 42,51 mA
 42,51 mA
 42,51 mA
 0 A

1 2 Δ 1/Δ Time Axis 18,59 s 24,63 s 6,038 s 165,6 mHz