



Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

Ref. No. : GEM/2026/B/7007849

Date: 03-02-2026

Bid Specific Terms and Conditions

WE ACCEPT ALL THIS ATC.

1. Generic

OPTION CLAUSE: The Purchaser reserves the right to increase or decrease the quantity to be ordered up to 25 percent of bid quantity at the time of placement of contract. The purchaser also reserves the right to increase the ordered quantity up to 25% of the contracted quantity during the currency of the contract at the contracted rates. The delivery period of quantity shall commence from the last date of original delivery order and in cases where option clause is exercised during the extended delivery period the additional time shall commence from the last date of extended delivery period. The additional delivery time shall be $(\text{Increased quantity} \div \text{Original quantity}) \times \text{Original delivery period (in days)}$, subject to minimum of 30 days. If the original delivery period is less than 30 days, the additional time equals the original delivery period. The Purchaser may extend this calculated delivery duration up to the original delivery period while exercising the option clause. Bidders must comply with these terms.

2. Generic

Bidder financial standing: The bidder should not be under liquidation, court receivership or similar proceedings, should not be bankrupt. Bidder to upload undertaking to this effect with bid.

3. Turnover

Bidder Turn Over Criteria: The minimum average annual financial turnover of the bidder during the last three years, ending on 31st March of the previous financial year, should be as indicated in the bid document. Documentary evidence in the form of certified Audited Balance Sheets of relevant periods or a certificate from the Chartered Accountant / Cost Accountant indicating the turnover details for the relevant period shall be uploaded with the bid. In case the date of constitution / incorporation of the bidder is less than 3 year old, the average turnover in respect of the completed financial years after the date of constitution shall be taken into account for this criteria.

4. Turnover

OEM Turn Over Criteria: The minimum average annual financial turnover of the OEM of the offered product during the last three years, ending on 31st March of the previous financial year, should be as indicated in the bid document. Documentary evidence in the form of certified Audited Balance Sheets of relevant periods or a certificate from the Chartered Accountant / Cost Accountant indicating the turnover details for the relevant period shall be uploaded with the bid. In case the date of constitution / incorporation of the OEM is less than 3 year old, the average turnover in respect of the completed financial years after the date of constitution shall be taken into account for this criteria. In case of bunch bids, the OEM of CATEGORY RELATED TO primary product having highest bid value should meet this criterion.

5. Service & Support

Availability of Service Centres: Bidder/OEM must have a Functional Service Centre in the State of each Consignee's Location in case of carry-in warranty. (Not applicable in case of goods having on-site warranty). If service center is not already there at the time of bidding, successful bidder / OEM shall have to establish one within 30 days of award of contract. Payment shall be released only after submission of documentary evidence of having Functional Service Centre.

6. Service & Support

Dedicated /toll Free Telephone No. for Service Support : BIDDER/OEM must have Dedicated/toll Free Telephone No. for Service Support.

7. Service & Support

Escalation Matrix For Service Support : Bidder/OEM must provide Escalation Matrix of Telephone Numbers for Service Support.

8. Certificates

Bidder's offer is liable to be rejected if they don't upload any of the certificates / documents sought in the Bid document, ATC and Corrigendum if any.

9. Certificates

ISO 9001: The bidder or the OEM of the offered products must have ISO 9001 certification.

Registered Office & Works: Plot No.27, Radha Nikunj B, Kharbas Circle, Sanganer, Jaipur-302020, Rajasthan. India

Web: www.starnuke.net, info@starnuke.net, sales@starnuke.net

Ph: +91-9950041555, 7073577706



Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

10. Past Project Experience

Proof for Past Experience and Project Experience clause: For fulfilling the experience criteria any one of the following documents may be considered as valid proof for meeting the experience criteria:a. Contract copy along with Invoice(s) with self-certification by the bidder that service/supplies against the invoices have been executed.b. Execution certificate by client with contract value.c. Any other document in support of contract execution like Third Party Inspection release note, etc.

Proof for Past Experience and Project Experience clause: For fulfilling the experience criteria any one of the following documents may be considered as valid proof for meeting the experience criteria:a. Contract copy along with Invoice(s) with self-certification by the bidder that service/supplies against the invoices have been executed.b. Execution certificate by client with contract value.c. Any other document in support of contract execution like Third Party Inspection release note, etc.

11. Past Project Experience

The Bidder / OEM {themselves or through reseller(s)}, should have executed project for supply and installation / commissioning of same or similar Category Products during preceding 3 financial years (i.e. current year and three previous financial years) as on opening of bid, as per following criteria:

- (i) Single order of at least 35% of estimated bid value; or
- (ii) Two orders of at least 20% each of estimated bid value; or
- (iii) Three orders of at least 15% each of estimated bid value.

Satisfactory Performance certificate issued by respective Buyer Organization for the above Orders should be uploaded with bid. In case of bunch bids, the Category related to primary product having highest bid value should meet this criterion

12. Forms of EMD and PBG

Bidders can also submit the EMD with Account Payee Demand Draft in favour of ADHO DANG payable at AHWA.

Bidder has to upload scanned copy / proof of the DD along with bid and has to ensure delivery of hardcopy to the Buyer within 5 days of Bid End date / Bid Opening date.

13. Forms of EMD and PBG

Successful Bidder can submit the Performance Security in the form of Account Payee Demand Draft also (besides PBG which is allowed as per GeM GTC). DD should be made in favour of ADHO DANG

payable at
AHWA

. After award of contract, Successful Bidder can upload scanned copy of the DD in place of PBG and has to ensure delivery of hard copy to the original DD to the Buyer within 15 days of award of contract.

14. Buyer Added Bid Specific ATC

Buyer uploaded ATC document Click here to view the file.

FOR STAR NUKE CONSULTING ENGINEERING SERVICES PVT LTD

Balram Singh Rajora
Managing Director





Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

Portable X - Ray Machine (V2) (Q2)

COMPLIANCE SHEET

GEM/2025/B/7007849

Dated: 03-02-2026

Sr. No.	Specification	Compliance
1.	General Description:*	
•	A high-frequency mobile X-ray system designed for bedside and emergency imaging, equipped with a spring-balanced arm and compact maneuverable design for indoor mobility.	YES
•	The unit shall be available in 3.5 kW, 4.2 kW, or 5.2 kW generator configurations.	YES
2.	X-Ray Generator:*	
•	Type: High-frequency X-ray generator	YES
•	Output Power Options: 3.5 kW / 4.2 kW / 5.2 kW	YES
•	X-ray Ripple Frequency: 100 kHz	YES
•	Input Power: Single phase, 220V, 50 Hz $\pm 10\%$, 15A	YES
•	Output Voltage Range: 40 – 125 kV	YES
•	mA Range: 40 – 100 mA	YES
•	Maximum mAs: 200 mAs	YES
3.	X-Ray Tube Assembly:*	
•	Tube Type: Stationary or Rotating anode (as per configuration)	YES
•	Focal Spot Size: 1.5 mm	YES
•	Tube Mount: Spring-balanced arm with folding feature for compact storage and easy mobility	YES
•	Tube Head Movement: 360° rotation with locking mechanism for precise positioning	YES
4.	Mobile Stand & Movement:*	
•	Design: Compact, lightweight with spring-balanced arm	YES
•	Hand Braking System for safe parking	YES
•	Easy movement on slopes, inclines, and ramps	YES
•	Big rear wheels and ergonomic handles	YES
•	Folding arm for space-saving and secure transport	YES
5.	Control Panel:*	
•	Type: Microprocessor-based digital feather-touch control panel	YES
•	Display: Integrated 14"/15" touchscreen LCD mounted on mobile stand	YES
•	APR (Anatomical Programmed Radiography): Yes, with body part and patient type presets	YES
•	Programmable Anatomical Technique: Adjustable by operator	YES
6.	Optional DR Upgrade:*	
•	Flat Panel Detector Compatibility: Upgradeable to Digital Radiography	YES
•	Panel Sizes Supported: 14" x 17" and 17" x 17"	YES
•	Wireless Transmission to Laptop	YES
•	Detector Type: Konica Minolta AeroDR or equivalent	YES
•	Pixel Size: 150 microns (NS or GS type)	YES



Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

7.	Safety & Compliance:*	
•	Radiation safety with collimator light and exposure controls	YES
•	Compliance: IEC and BIS/CE certification (as applicable)	YES
•	AERB type approval (mandatory in India)	YES
•	Emergency stop button and overload protection circuit	YES
8.	Accessories (Mandatory):*	
•	Cassette storage compartment	YES
•	Power cord and charger	YES
•	Collimator with light source	YES
•	Operator and service manuals	YES
•	Optional wireless detector and laptop for DR use	YES

Balram Singh Rajora
Director & CEO
ceo@starnukemail.net






राजस्थान/RAJASTHAN

S 481579



DECLARATION OF NON-BLACKLISTING

I, Balram Singh Rajora do hereby solemnly affirm and declare as under representing T of M/S STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED JAIPUR as do hereby certify that our company has not been found guilty of malpractice or misco not been blacklisted or debarred by the Public Health Department or by any Tender In The firm has also not been blacklisted by any State Government or Central Governmen Organization/Bank, nor on the GeM portal. We further confirm that our firm has not b have any adverse observations been made against it by any Government Department

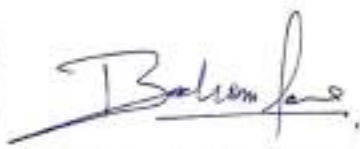

Balram Singh Rajora
Director & CEO
ceo@starnukemail.net



विजयवायु स्टेशन अधिनियम, 1954	
स्टेशन राशि पर प्रयोजित अंश	
1. आधारभूत आवश्यकता सुविधाओं के लिए (घांटा 3-क) - 10% अंश	50
2. भाग और पदवी प्राप्त के दौरान और बाद के लिए (घांटा 3-क) / प्रत्येक वर्ष के लिए एवं अन्य निर्दिष्ट आवश्यकता के लिए - 20% अंश	100
कुल अंश प्रति एक घंटा घंटा दर	150

क्रमांक 5489 दिनांक 19 FEB 2025

प्रेता का नाम HD FC

पिता का नाम

मार्क मरीन L W

निवासी

मुद्रांक मुद्रा

500 दिनांक 19 FEB 2025

कस्टो

राज्य सरकार
स्टेशन दिनांक 19/02/25
राज्य सरकार





Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

GeM No. GEM/2026/B/7007849

Date : 03/02/2026

DECLARATION We solemnly declare that we have attached all the documents mentioned here above and mentioned in the tender . We also understand that non-compliance of any documents will be treated as non-respective Tender and we will lose our claim to participate in the tender Enquiry automatically and our tender will be liable to rejected

For Star Nuke Consulting Engineering Services Pvt. Ltd



Balram Singh Rajora
Managing Director
ceo@starnukemail.net



Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

Date: 03-02-2026

LATEST ART OF TECHNOLOGY

GEM Bid No. : GEM/2026/B/7007849

Dated: 03-02-2026

We, M/s. Star Nuke Consulting Engineering Services Pvt. Ltd. Plot No. 27, Radha Nikunj B, Kharbas Circle, Sanganer, Jaipur-302020, Rajasthan. India, established & reputable manufacturer of the medical devices listed hereunder, do hereby confirm that we are manufacturing Portable X Ray Machine in our ISO 13485 certified and AERB approved facility as per the technical details provided by GEM.

We certify and Portable X Ray Machine is our latest art of technology machine.

Product Name: Portable X Ray Machine

Model name : HF-100

For Star Nuke Consulting Engineering Services Pvt. Ltd



Balram Singh Rajora
Managing Director
ceo@starnukemail.net



Star Nuke Consulting Engineering Services Private Limited
AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

Bidder Financial Standing

Ref. No. : GEM/2026/B/7007849

Date: 03-02-2026

I Balram Singh Rajora do hereby solemnly affirm and declare as under:-

1. That I am MD of M/S STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED.

1.Bidder financial standing: We have not been under liquidation, court receivership or similar proceedings and is not bankrupt.

(a) STAR NUKE is never blacklisted and no litigation/court case pending in this regard.

2. Track record of M/S STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED is clean and is not in any involvement in illegal activities or financial frauds. There is no case with the Police/Court/Regulatory authorities against us.

3. We have not been prosecuted or suffered any penalty for violation of any statutory laws by any Authority.

4. We have not been suspended / delisted / blacklisted by any organization on any grounds.

5. We have not been rescinded/abandoned any contract awarded by any of his clients before the expiry of prescribed period of contract.

Verified that the contents of my above affidavit are true to the best of my knowledge and belief and nothing has been concealed there in.

FOR STAR NUKE CONSULTING ENGINEERING SERVICES PVT LTD

Balram Singh Rajora
Managing Director





Star Nuke Consulting Engineering Services Private Limited
AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

Ref. No. : GEM/2026/B/7007849

Date: 03-02-2026

I Balram Singh Rajora do hereby solemnly affirm and declare as under:-

1. That I am MD of M/S STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED.
2. That we undertake to supply spare parts for smooth functioning of the quoted specified equipment if needed (For Tender Bid No. GEM/2026/B/7007849) for 10 years from the date of purchase.

Verified that the contents of my above affidavit are true to the best of my knowledge and belief and nothing has been concealed there in.

FOR STAR NUKE CONSULTING ENGINEERING SERVICES PVT LTD

Balram Singh Rajora
Managing Director



Registered Office & Works: Plot No. 27, Radha Nikunj B, Kharbas Circle, Sanganer, Jaipur, Rajasthan, 302020

Web: www.starnuke.net, info@starnuke.net, sales@starnuke.net

Ph: +91-9950041555, 7073577706



Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

WARRANTY CERTIFICATE

GeM No. GEM/2026/B/7007849

Date : 03/02/2026

We Accept,

Warranty period of the supplied products shall be 1 year and CAMC will be @10 % Yearly from the date of final acceptance of goods or after completion of installation, commissioning & testing of goods (if included in the scope of supply), at consignee location. We guarantee the rectification of goods in case of any break down during the guarantee period. we have well established Installation, Commissioning, Training ,Troubleshooting and Maintenance Service group in INDIA for attending the after sales service.

For Star Nuke Consulting Engineering Services Pvt. Ltd


Balram Singh Rajora
Managing Director
ceo@starnukemail.net





Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

Dear Sir,

Ref: Your Bid document No GEM/2026/B/7007849

Dated 03/02/2026

The seller should upload following certificate in the bid:

(a) This is to certify that the Hardware and the Software being offered, as part of the contract, does not contain Embedded Malicious code that would activate procedures to :

- (i) Inhibit the desires and designed function of the equipment.
- (ii) Cause physical damage to the user or equipment during the exploitation.
- (iii) Tap information resident or transient in the equipment/network.

(b) The firm will be considered to be in breach of the procurement contract, in case physical damage, loss of information or infringements related to copyright and Intellectual Property Right (IPRs) are caused due to activation of any such malicious code in embedded software.

FOR STAR NUKE CONSULTING ENGINEERING SERVICES PVT LTD



Balram Singh Rajora
Managing Director
ceo@starnukemail.net

INDIAN INCOME TAX RETURN ACKNOWLEDGEMENT [Where the data of the Return of Income in Form ITR-1(SAHAJ), ITR-2, ITR-3, ITR-4(SUGAM), ITR-5, ITR-6, ITR-7 filed and verified] (Please see Rule 12 of the Income-tax Rules, 1962)			Assessment Year 2024-25
PAN	AAVCS3158D		
Name	STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED		
Address	25 , Navkar Nagar,Kalyanpura Sanganer , Jaipur , 27-Rajasthan, 91-INDIA, 302020		
Status	7-Private company	Form Number	ITR-6
Filed u/s	139(1)-On or before due date	e-Filing Acknowledgement Number	640940251241024
Taxable Income and Tax Details	Current Year business loss, if any	1	0
	Total Income	2	1,93,33,280
	Book Profit under MAT, where applicable	3	0
	Adjusted Total Income under AMT, where applicable	4	0
	Net tax payable	5	48,65,800
	Interest and Fee Payable	6	5,03,388
	Total tax, interest and Fee payable	7	53,69,188
	Taxes Paid	8	53,69,193
	(+) Tax Payable /(-) Refundable (7-8)	9	(-) 10
Accreted Income and Tax Detail	Accreted Income as per section 115TD	10	0
	Additional Tax payable u/s 115TD	11	0
	Interest payable u/s 115TE	12	0
	Additional Tax and interest payable	13	0
	Tax and interest paid	14	0
	(+) Tax Payable /(-) Refundable (13-14)	15	0
Income Tax Return electronically transmitted on 24-Oct-2024 18:24:39 from IP address 49.36.238.204 and verified by usha rao having PAN AJSPR3638Q on 24-Oct-2024 using paper ITR-Verification Form /Electronic Verification Code generated through mode			
System Generated Barcode/QR Code	 AAVCS3158D0664094025124102495256be44698cb460364814431e73b0c41eff72e		
DO NOT SEND THIS ACKNOWLEDGEMENT TO CPC, BENGALURU			

INDIAN INCOME TAX RETURN ACKNOWLEDGEMENT

Assessment Year

[Where the data of the Return of Income in Form ITR-1 (SAHAJ), ITR-2, ITR-3, ITR-4 (SUGAM), ITR-5, ITR-6, ITR-7 filed and verified]
(Please see Rule 12 of the Income-tax Rules, 1962)

2022-23

PAN AAVCS3158D

Name STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED

Address 25, Navkar Nagar, Kalyanpura Sangarner, Jaipur, 27-Rajasthan, 91-INDIA, 302020

Status Pvt Company

Form Number

ITR-6

Filed u/s 139(1)-On or before due date

e-Filing Acknowledgement Number 745319621221022

Taxable Income and Tax details	Current Year business loss, if any	1	0
	Total Income		11,70,830
	Book Profit under MAT, where applicable	2	12,96,427
	Adjusted Total Income under AMT, where applicable	3	0
	Net tax payable	4	2,02,243
	Interest and Fee Payable	5	0
	Total tax, interest and Fee payable	6	2,02,243
Accreted Income & Tax Details	Taxes Paid	7	4,88,064
	(+) Tax Payable / (-) Refundable (6-7)	8	(-) 2,85,820
	Accreted Income as per section 115TD	9	0
	Additional Tax payable u/s 115TD	10	0
	Interest payable u/s 115TE	11	0
	Additional Tax and interest payable	12	0
	Tax and interest paid	13	0
	(+) Tax Payable / (-) Refundable (12-13)	14	0

This return has been digitally signed by NSULTING ENGINEERING SERVICES PR in the capacity of Director havingPAN AJSPR3638Q from IP address 103.175.172.42 on 22-Oct-2022 DSC SI No & Issuer 2938635775206337198& 2938635775206337198CN=SafeScrip sub-CA for RCAI Class3 2014,OU=Sub-CA,O=Sify Technologies Limited,C=IN

System Generated

Barcode/QR code

AAVCS3158D067453196212210221b48d96c48f204df23b20d76de06c36c040c66c

DO NOT SEND THIS ACKNOWLEDGEMENT TO CPC, BENGALURU

verified as per records available on IncomeTax Portal.

Sukhpreet



INDIAN INCOME TAX RETURN ACKNOWLEDGEMENT

(Where the data of the Return of Income in Form ITR-1(SAHU), ITR-2, ITR-3, ITR-4(SUGAM), ITR-5, ITR-6, ITR-7 filed and verified)
(Please see Rule 12 of the Income-tax Rules, 1962)

Assessment
Year
2023-24

PAN	AAVCS3158D		
Name	STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED		
Address	25, Navkar Nagar, Kalyanpura Sanganer, Jaipur, 27-Rajasthan, 91-INDIA, 302020		
Status	7-Private company	Form Number	ITR-6
Filed u/s	139(1)-On or before due date	e-Filing Acknowledgement Number	437976291251023

Taxable Income and Tax Details	Current Year business loss, if any	1	0
	Total Income	2	9,44,310
	Book Profit under MAT, where applicable	3	9,95,821
	Adjusted Total Income under AMT, where applicable	4	0
	Net tax payable	5	1,55,348
	Interest and Fee Payable	6	0
	Total tax, interest and Fee payable	7	1,55,348
Accreted Income and Tax Detail	Taxes Paid	8	6,79,171
	(+) Tax Payable /(-) Refundable (7-8)	9	(-) 5,23,820
	Accreted Income as per section 115TD	10	0
	Additional Tax payable u/s 115TD	11	0
	Interest payable u/s 115TE	12	0
	Additional Tax and interest payable	13	0
	Tax and interest paid	14	0
	(+) Tax Payable /(-) Refundable (13-14)	15	0

Income Tax Return submitted electronically on 25-Oct-2023 13:44:12 from IP address 49.36.233.76 and
verified by usha rao having PAN AJSPR3638Q on 25-Oct-2023 using paper ITR-
Verification Form /Electronic Verification Code _____ generated through mode

System Generated

Barcode/QR Code



AAVCS3158D06437976291251023338ec5718ea49acdb0b63daf73ad510009c9f2d5

DO NOT SEND THIS ACKNOWLEDGEMENT TO CPC, BENGALURU

verified as per details on Income Tax Portal

Usha Rao





Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

Date: 03-02-2026

MANUFACTURER'S AUTHORISATION

GEM Bid No. : GEM/2026/B/7007849

Dated: 03-02-2026

We, M/s. Star Nuke Consulting Engineering Services Pvt. Ltd. Plot No. 27, Radha Nikunj B, Kharbas Circle, Sanganer, Jaipur-302020, Rajasthan, India, established & reputable manufacturer of the medical devices listed hereunder, do hereby confirm that we are manufacturing Portable X Ray Machine in our ISO 13485 certified and AERB approved facility as per the technical details provided by GEM.

We authorize ourselves, M/s Star Nuke Consulting Engineering Services Pvt. Ltd to submit the proposal, do sales, negotiate, close order and undertake service & market development for Portable X Ray Machine against the bid number GEM/2026/B/7007849 Dated: 03-02-2026 and also against other enquiries in entire India.

Product Name: Portable X Ray Machine

Model name: HF-100

This authorization letter is valid until: 31st December 2026.

For Star Nuke Consulting Engineering Services Pvt. Ltd

Balram Singh Rajora
Managing Director
ceo@starnukemail.net





केस फाइल नं. Case File Number: RJ-82197-MF-XRE-001

जारी करने की तिथि Issuance Date: 17/05/2022

समाप्ति की तिथि Document Number: 22-TA-775873

समाप्ति की तिथि Expiry Date: 17/05/2025

**STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED, JAIPUR, INDIA द्वारा
निर्मित STARNUKE-HF100 द्वारा निर्मित RADIOGRAPHY (MOBILE) के लिए टाइप अनुमोदन
TYPE APPROVAL FOR RADIOGRAPHY (MOBILE) EQUIPMENT MODEL STARNUKE-HF100
MANUFACTURED BY STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE
LIMITED, JAIPUR, INDIA**

परमाणु ऊर्जा अधिनियम, 1962 की धारा 16 के तहत प्रदत्त शक्तियों का प्रयोग करते हुए, परमाणु ऊर्जा (विकिरण संरक्षण) नियम 2004 के नियम 3 को पढ़ें, परमाणु ऊर्जा नियामक परिषद् (एईआरबी) एतद्वारा रेडियोलॉजिकल संरक्षा दृष्टिकोण से निम्नलिखित चिकित्सा नैदानिक एक्स-रे उपकरण को टाइप अनुमोदन जारी करता है।

In exercise of the powers conferred under Section-16 of the Atomic Energy Act, 1962 read in conjunction with Rule-3 of the Atomic Energy (Radiation Protection) Rules, 2004, the Atomic Energy Regulatory Board (AERB) hereby grants Type Approval to following medical diagnostic x-ray equipment from radiological safety view point:

उपकरण का प्रकार Type of Equipment	Radiography (Mobile)
मॉडल का नाम Model Name	STARNUKE-HF100
विनिर्माता का नाम Name of Manufacturer	STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED, India
एक्स-रे ट्यूबों की सं. No. of x-ray tubes	1
महत्तम प्रचालित वोल्टेज Maximum operating voltage	100.000 kVp
महत्तम प्रचालित करंट Maximum operating current	100.000 mA

नियम एवं शर्तें TERMS AND CONDITIONS

1. इन नियमों और शर्तों को आपूर्तिकर्ता के प्राधिकरण के नियमों और शर्तों के संयोजन में पढ़ा जाना चाहिए। संभावित उपयोगिता को इस प्रकार की स्वीकृति और आपूर्तिकर्ता के प्राधिकरण की एक प्रति प्रदान की जाएगी। These Terms and Conditions to be read in conjunction with Terms and Conditions of Supplier's Authorization. A copy this Type Approval and Supplier's Authorization shall be provided to the prospective utility.
2. इन नियमों और शर्तों को आपूर्तिकर्ता के प्राधिकरण के नियमों और शर्तों के संयोजन में पढ़ा जाना चाहिए। संभावित उपयोगिता को इस प्रकार की स्वीकृति और आपूर्तिकर्ता के प्राधिकरण की एक प्रति प्रदान की जाएगी। This Type Approval becomes invalid if any change is made in the design of above model.
3. उपकरण खरीदने के लिए एईआरबी से आवश्यक अनुमति प्राप्त करने वाले यूजर को ही टाइप अनुमोदित मॉडल की आपूर्ति की जाएगी। The Type Approved Model shall be supplied only by Suppliers Authorised by AERB and to the user who has obtained requisite permission from AERB to procure the equipment.
4. आपूर्तिकर्ता एक्स-रे उपकरण की स्थापना और कमीशनिंग के बाद उपयोगिता को गुणवत्ता आश्वासन परीक्षण रिपोर्ट के साथ मुहर सहित विधिवत हस्ताक्षरित स्थापना रिपोर्ट प्रदान करेगा। Supplier shall provide duly signed and stamped installation report with Quality Assurance test report to utility after installation and commissioning of x-ray equipment.
5. इस टाइप अनुमोदन की समाप्ति के बाद कथित मॉडल की आपूर्ति इसके पुनर्वैधीकरण पर सशर्त है। The supply of above Model after expiry of this Type Approval is conditional upon its revalidation.

(सक्षम प्राधिकारी Competent Authority)

MRS. USHA RAO

STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED

PLOT NO 25, NAVKAR NAGAR, OPP. TO MANSAROVAR RICCO KANTA, NEW SANGANER ROAD VIALLGE
KALYANPURA, TEHSIL SANGANER JAIPUR, RAJASTHAN-302020

BUREAU OF INDIAN STANDARDS

Attachment to Licence No. CM/L- 8400193016

CM/L-No	Name of the Licensee with the Factory Address	Name of the Product	Indian Standard No.
8400193016	Star Nuke Consulting Engineering Services Pvt Ltd -PLOT NO 27, RADHA NIKUNJ-B, AT KHARBAS CIRCLE, NEAR HOTEL HAYAT RESIDENCY, , MANSAROVAR , Jaipur : 302020	Diagnostic Medical X-ray Equipment - Part 1 : General and Safety Requirements	IS 7620 : PART 1 : 1986

Endorsement No. 9 Dated 03-Nov-2025

Whereas, the licence was valid upto Eleventh January Two Thousand Twenty Six.

Now, consequent upon renewal, the validity of the licence given in schedule of the Licence Dated 10-JAN-2026 has been extended from Eleventh January Two Thousand Twenty Six to Tenth January Two Thousand Thirty

Other terms and conditions of licence remain same.

Branch Head (Jaipur Branch Office)



भारतीय मानक ब्यूरो
BUREAU OF INDIAN STANDARDS

जयपुर शाखा कार्यालय-I
Jaipur Branch Office-I

Address: Manak Bhawan
Prithviraj Road, C-Scheme- Jaipur-302005

दूरभाष (Phones): 0141-2223282, 2223283, 2223284

फैक्स (Fax): 0141-2223286

ई-मेल (e-mail): jpbis@bis.gov.in

वेब (web): <http://www.bis.org.in>

हमारा संदर्भ JBO/एल-8400193016

दिनांक 05/04/2022

M/s Star Nuke Consulting Engineering Services Pvt Ltd,
Plot No 25, Navkar Nagar, Kalyanpura, New Sanganer Road,
Sanganer, Distt.:Jaipur (Rajasthan)-302020

महोदय(यों),

भा मा ब्यूरो प्रमाणन मुहर लाइसेंस संख्या सीएम/एल-8400193016 के संदर्भ में है जिसे आपने Diagnostic Medical X-ray Equipment - Part 1 : General and Safety Requirements IS 7620 (Pt.1) : 1986 के अनुसार है, जो 10/01/2023 तक वैध है।

हमें आपको यह सूचित करते हुए हर्ष है कि भा मा ब्यूरो ने आपके लाइसेंस में दिनांक 07-03-2022 से नई किस्म समाविष्ट करने के लिए सहमति दे दी है।।

जब और जहाँ नई किस्म के मुहरांकन को शुरू करते हैं, कृपया हमें सूचित करें। आपको सलाह दी जाती है कि उक्त किस्म का एसआईटी के अनुसार परीक्षण करने के उपरांत अलग से रिकार्ड रखें।

नई किस्म के लिए पृष्ठांकन शीट संख्या 1 संलग्न है।

सधन्यवाद,

भवदीय,
कनिका
(कनिका कालिया)
वैज्ञानिक 'ई' एवं प्रमुख



भारतीय मानक ब्यूरो BUREAU OF INDIAN STANDARDS

उपभोक्ता मामले, खाद्य एवं सार्वजनिक वितरण मंत्रालय,
भारत सरकार

Ministry of Consumer Affairs, Food and Public
Distribution, GOVT. OF INDIA

जयपुर शाखा कार्यालय-1

Jaipur Branch Office-I

पता/Address: मानक भवन, पृथ्वीराज रोड,

सी-स्कीम, जयपुर-302005

Manak Bhawan, Prithviraj Road

C-Scheme, Jaipur, 302005

दूरभाष/Phones: 0141-2223282, 2223283, 2223284

फैक्स/fax: 0141-2223281

ई-मेल/E-Mail: jpbo@bis.gov.in

वेबसाइट/web: <http://www.bis.org.in>

लाइसेंस संख्या सी एम/एल- 8400193016 की संलग्नी
ATTACHMENT TO LICENCE NO. CM/L- 8400193016

सी एम/एल संख्या CML/NO	लाइसेंसधारी का पता सहित नाम NAME OF THE LICENSEE WITH THE ADDRESS	उत्पाद का नाम NAME OF THE PRODUCT	भा मा संख्या IS NO.
8400193016	M/s Star Nuke Consulting Engineering Services Pvt Ltd, Plot No 25, Navkar Nagar, , Kalyanpura, New Sanganer Road, Sanganer, Distt.:Jaipur (Rajasthan)- 302020,	Diagnostic Medical X-ray Equipment - Part 1 : General and Safety Requirements	IS 7620 : PART 1:1986

पृष्ठांकन संख्या 1 दिनांक Dated: 05/04/22
ENDORSEMENT NO. 1 DATED

निम्न अतिरिक्त (आकारों/प्रकारों/श्रेणियों, आदि) लाइसेंस के प्रथम अनुसूची के कालम (2) में और द्वितीय अनुसूची के कालम (1) में प्रथम अनुसूची के कालम (1) में मानक मुहर सहित दिनांक 07-03-2022 से प्रभावी होने के साथ सम्मिलित किया जाता है।

The following additional (sizes/types/grades etc.) has (have) been included in Columns(2) of the first schedule and column (1) of the the Second Schedule of the Licence alongwith the Standard Mark in Column (1) of First Schedule with effect from 07-03-2022

1. Diagnostic X-ray machine Permanently Installed type, Six Pulse Line Frequency Generator, For rated line voltage 230 + 10 V, frequency 50 Hz, Three phase, Current 300 mA, Rated Peak Output Voltage 125 kVp, Output power 24 kW with Horizontal Bucky Table.
2. Diagnostic X-ray machine Stationary type, High frequency generator, For rated line voltage 230 V, frequency 50 Hz, Single phase, Output Current 100 mA, Rated Peak Output Voltage 110 kV, Output power 5 KW with Horizontal Bucky Table.
3. Diagnostic X-ray machine Mobile type, High frequency generator, For rated line voltage 230 V, frequency 50 Hz, Single phase, Output Current 100 mA, Rated Peak Output Voltage 110 kV, Output power 5 KW .
4. Diagnostic X-ray machine Stationary type, High frequency generator, For rated line voltage 230 V, frequency 50 Hz, Single phase, Output Current 320 mA, Rated Peak Output Voltage 125 kV, Output power 20 KW with Horizontal Bucky Table.
5. Diagnostic X-ray machine Portable Handheld Dental, For rated line voltage 240 V, 50 Hz Single Phase, Current 2.5 mA, Rated Peak voltage 65 kV, Output Power 162.5 W High Frequency Generator

लाइसेंस की अन्य निबन्धन व शर्तें यथावत हैं।

Other terms and conditions of Licence remain the same.

कनिष्ठा
(कनिष्ठा कालिमा)
वैज्ञानिक 'ई' एवं प्रमुख

CERTIFICATE



No. 0P250304.SNCU083

Test Report / Technical Construction File no. TLHK25022867452 TEHK25022867453

Certificate's
Holder:

STAR NUKE CONSULTING ENGINEERING SERVICES
PRIVATE LIMITED

Plot no. 27, Radha Nikunj-B, Iskcon Road, Near Hotel Hayatt
Regency, Kharbas Circle, Mansarovar, Jaipur, Rajasthan,
302020, India.

Certification
ECM Mark



Product:

Flat Panel detector (Wired and Wireless)

Model(s):

STARNUKE4343DI, STARNUKE4343DIW, STARNUKE3543DI,
STARNUKE3543DIW

Verification to:

Standard:

EN 61010-1:2010+A1:2019, EN IEC 61326-1:2021

related to CE Directive(s):

2014/35/EU (Low Voltage)

2014/30/EU (Electromagnetic Compatibility)

Remark:

The manufacturer has voluntarily decided to submit its documents concerning the above-mentioned product for verification. Ente Certificazione Macchine confirms that the documentation made available and immediately returned to it, as containing sensitive data, meets the essential requirements of the above-mentioned directive/standard. The verification activity carried out exclusively concerned the technical documentation and no verification was carried out on the product. This document cannot replace the EC Declaration of Conformity. This document was issued in accordance with regulation RGVOL01 published on the website of www.entecerma.it and concerning voluntary certifications with a non-notified procedure.

Issuance date: 04 March 2025

Expiry date: 03 March 2030

For online check:



Approver

Ente Certificazione Macchine
Legal Representative
Luca Bedonni



Mobile X-Ray Machine

STARNUKE-HF100



Components



Tube Head



**Exposure Hand
Switch**



Operational panel



Laptop Stand

Technical Specifications



Feature	Detail / Value
Model Name	STARNUKE-HF100
Application / Usage	General Radiography
X-Ray Generator Type	High Frequency
X-Ray Generator Power	5.6 kW
X-Ray Beam Energy (kV Range)	40-125 kV
X-Ray Tube Current (mA Range)	5-100 mA
Exposure Time Range	0.01ms –10000ms
Focal Spot Size (Small)	0.6 mm
Focal Spot Size (Large)	1.8 mm
Max. Permissible mAs	0.1-320 mAs
Tube Heat Storage Capacity	30 KJ
Anode Type	Stationary
SID (Centimeter)	100 cm
Total Filtration (mm Al Equivalent)	2.8 mm Al
Power Requirements	230 VAC 50 Hz, Single Phase

Certification & Approvals

1. CDSCO Approved X-Ray Generator
2. AERB Type Approved X-Ray Device
3. Certified under BIS - IS 7620: Part 1: 1986
4. ISO 13485 Certified Manufacturing Facility
5. NABL Accredited Laboratory with ISO 17025:2017 Quality Management System
6. Certified OEM by QCI at GEM for Make in India products

Contact us

Ph. No. +91-7073577706

Email: info@starnukemail.net

www.starnuke.net




Digital Radiography Panel

STARNUKE 4343DIW



Components

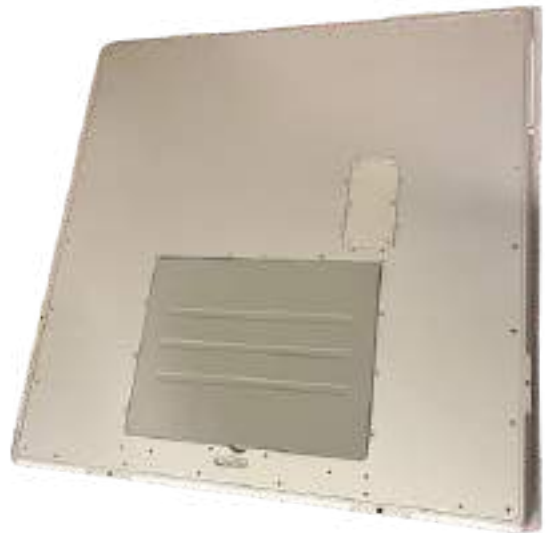

DR DETECTOR FRONT AND BACK



BATTERY

BATTERY CHARGER

Technical Specifications

Model	STARNUKE4343DIW
Scintillator	CsI:TI (Direct)
Detector Technology	IGZO
Pixel Matrix	3072 x 3072
Pixel Size / Pixel Pitch	140 μ m
X-Ray Beam Energy Voltage Range	40 ~ 150 kVp
Spatial Resolutions	3.4 lp/mm
A/D Conversion	16 bits
DQE	82 % at 0.5 lp/mm
MTF	87 % at 0.5 lp/mm
Image Acquisition Time	2.0 Secs
Battery Stand by Time	8 Hours
Data Interface	Giga Ethernet (1000BaseT), Wi-Fi (802.11 ac, 2.4/5 GHz)
Communication Mode	Wired / Wireless
Adaptor Input	100-240 V ~50/60Hz 1.5 A
Adaptor output	15V 4.0A
Water Resistance	IP68
Operating Environment	T(10~+40) / H(20 ~ 75%) / P(70~160KPa)
Image Storage	1000 Images
Load bearing Capacity	200 Kg
Mobile Operation Mode / View	Yes, Through Android App
Drop Test	1 meter



Contact us

Ph. No. +91-7073577706

Email: info@starnukemail.net

www.starnuke.net



Star Nuke Consulting Engineering Services Private Limited

AERB (Govt. of India) Authorized - ISO 9001-2015 Certified company

ESCALATION MATRIX FOR SERVICE SUPPORT

The service center details of **STAR NUKE CONSULTING ENGINEERING SERVICES PVT LTD**, is given below:

Registered Office & Works: Gali No – 36 , F/F C-146 , Mahavir Enclave –III , Delhi , West Delhi, 110059

Registered Office & Works: Plot No. 27, Radha Nikunj B, Kharbas Circle, Sanganer, Jaipur-302020, Rajasthan.

Registered Office & Works: Plot No. F410, Raja ji Puram, Near Ayurvedic Hospital, Avas Vikas Colony, Lucknow , Uttar Pradesh , 226017

Registered Office & Works : Village- Leti , Post – Jaulkande, District –Bageshwar, Uttarakhand , 263642

Registered Office & Works : Shop No. 018/10, Ground Floor , Pala Building , Empire Industrial Centrum , Kalyan-Badlapur , Chikholi , Ambarnath(W) Thane, 421505

Registered Office & Works : C-141I, SECTOR-11A, KAMAL VIHAR, RAIPUR, Raipur, Chhattisgarh, 492001.

Registered Office & Works : 105/12, Seal Colony, Dum Dum Road, Kolkata , North 24 Parganas, West Bengal , 700074

Registered Office & Works : Kalwa Chowk, 2nd, 210, Shikhar Complex, Jayshree Road, Talab Darwaja, Junagadh, Junagadh, Gujarat, 362001

Registered Office & Works : Diyasai Arcade, 12-7-140/2, Anjaneya Nagar, AGI Colony, Moosapet, Hyderabad, Telangana 500018

Registered Office & Works : Plot no 184, Synergy Regancy, Gokul Nagar ,Indore, 452016. Madhya Pradesh

Registered Office & Works : No.160/2 , 1ST Floor, Sultanpet , Bengaluru , 560053

Registered Office & Works : Radium Road , Ranchi -834001 , Jharkhand

Registered Office & Works : 61, VIP Road, Near Tennis Stadium, Sachal, Guwahati – 781022, Assam

Registered Office & Works : Tenga Medical Store ,Tenga Market ,Tenga, Arunachal Pradesh

Registered Office & Works : GROUND FLOOR, D 30, Ramhlun NORTH BASIC MUAL, Aizawl, Mizoram, 796001

Escalation Matrix for service support	Level-1 BHAGAT SINGH (TECHNICAL ENGINEER) : 6375602671
	Level-2 AKSHITA SHARMA (TECHNICAL ENGINEER) :6375604173
	Level-3 TOLL FREE NO.- 0141-6764685

FOR STAR NUKE CONSULTING ENGINEERING SERVICES PVT LTD

Balram Singh Rajora
Managing Director



Registered Office & Works: Plot No. 27, Radha Nikunj B, Kharbas Circle, Sanganer, Jaipur, Rajasthan. India

Web: www.starnuke.net , info@starnuke.net , sales@starnuke.net

Ph: +91-9950041555, 7073577706



FORM MD-9

[See sub-rule (1) rule 25]

Licence to Manufacture for Sale or for Distribution of Class C or Class D medical device

Licence Number: MFG/MD/2023/001000

1. M/s STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED, PLOT NO. 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANERSANGANER, Jaipur, Rajasthan (India) - 302020 Telephone No.: 1416764685 FAX: 1416764685 has been licenced to manufacture for sale or for distribution the below listed medical device(s) at the premises situated at M/s STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED, Plot No 25, Navkar Nagar, Jaipur, Rajasthan (India) - 302020 Telephone No.: 1416764685, 9950041555 FAX: 1416764685

2. Details of medical device(s) [Annexed]

3. The names, qualifications and experience of the competent technical staff responsible for the manufacture and testing of the above mentioned medical device(s): As per records maintain by the manufacturer

4. This licence is subject to the provisions of the Medical Devices Rules, 2017 and conditions prescribed therein.

ANNEXURE

S.No.	Details Of Device(s)
-------	----------------------

RAJEEV SINGH
RAGHUVANS
HI

Digitally signed by RAJEEV SINGH RAGHUVANSHI
DN: c=IN, o=CENTRAL DRUGS STANDARD CONTROL
ORGANIZATION, ou=RAJEEV SINGH RAGHUVANSHI,
2.5.4.20=80c62f6a23e4eafbe8a239774cdeb03c27690
41015a06564f667f54b765db1cb,
postalCode=600034, st=TAMIL NADU,
serialNumber=657F5E47D940085D8F03BDC902D0E1
FET3CFA12A1A126EA94F5701124A19013,
cn=RAJEEV SINGH RAGHUVANSHI
Date: 2023.11.28 14:35:23 +05'30'

1	Generic Name:Dental Handheld X-Ray Machine HF Model No.:Ai Ray - Diagnostic X-ray machine Portable Handheld Dental For rated line voltage 240 V frequency 50 Hz Single Phase Current 2.5 mA Rated Peak voltage 65 kVp Output Power 162.5 W High Frequency Generator ,V-Light Eco - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 60 kV Output Power 120 W High Frequency Generator ,STARNUKE-DNTX - Diagnostic X-ray machine Portable Handheld Dental For rated line voltage 240 V frequency 50 Hz Single Phase Current 2.5 mA Rated Peak voltage 65 kVp Output Power 162.5 W High Frequency Generator ,Mini Ray - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator ,Ai-Ray - Diagnostic X-ray machine- Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 3 mA Rated Peak voltage 70 kV Output Power 210 W High Frequency Generator ,Waldent V-Light Eco - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 60 kV Output Power 120 W High Frequency Generator ,i-lite - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator , Starlite Eco - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 60 kV Output Power 120 W High Frequency Generator Intended Use:The use of Dental X-Ray Machine is to detect oral health issues, like cavities and gum disease, before they worsen. Class of medical device:Class C Material of construction:Fiber Plastic Dimension(if any): Shelflife:15 Years Sterile or Non sterile:Non-Sterilized Brand Name(if registered under the Trade Marks Act, 1999):STARNUKE
---	---

RAJEEV SINGH
RAGHUVANSHI
 I

Digitally signed by RAJEEV SINGH RAGHUVANSHI
 DN: cn=RAJEEV SINGH RAGHUVANSHI, o=CENTRAL DRUGS STANDARD CONTROL
 ORGANIZATION, ou=RAJEEV SINGH RAGHUVANSHI,
 2.5.4.20=80c62f6a23e4eafbe8a239774cdeb03c27690
 41015a06564fe67f54b765db1cb,
 postalCode=600034, st=TAMIL NADU,
 serialNumber=65775E47D940985D8F03BDC902D0E1
 FE73CFA12A1A126EA94FA5701124A19013,
 cn=RAJEEV SINGH RAGHUVANSHI
 Date: 2023.11.28 14:35:39 +05'30'

2	Generic Name:X-Ray Machine Radiography (Fixed) HF Model No.:STARNUKE-HF100R - Diagnostic X-ray machine Fixed type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100mA Rated Peak Output Voltage 110kVp Output power 5KW with Table ,STARNUKE-HF300 - Diagnostic X-ray machine Stationary type High frequency generator For rated line voltage 230 V frequency 50 Hz three phase Output Current 320 mA Rated Peak Output Voltage 125 kVp Output power 20 KW with Table ,STARNUKE-HF100R Digital Radiography System - Diagnostic Digital Radiography System Stationary type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 110 kVp Output power 5 KW with Table ,STARNUKE-HF300 Digital Radiography System - Diagnostic Digital Radiography System Stationary type High frequency generator For rated line voltage 230 V frequency 50 Hz three phase Output Current 320 mA Rated Peak Output Voltage 125 kVp Output power 20 KW with Table Intended Use:It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. Class of medical device:Class C Material of construction:Metal Body Dimension(if any): Shelflife:15 Years Sterile or Non sterile:Non-Sterilized Brand Name(if registered under the Trade Marks Act, 1999):STARNUKE
3	Generic Name:X-Ray Machine Radiography (Portable) HF Model No.:MINE 2IN - Diagnostic X-ray machine Portable Handheld Battery Operated for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator ,MIN-X - Diagnostic X-ray machine Portable Handheld Battery Operated for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator ,MIN-X Portable Digital Radiography System - Diagnostic Digital Radiography System Portable Handheld Battery Operated for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator Intended Use:It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. Class of medical device:Class C Material of construction:Metal Body Dimension(if any): Shelflife:15 Years Sterile or Non sterile:Non-Sterilized Brand Name(if registered under the Trade Marks Act, 1999):STARNUKE

RAJEEV SINGH
RAGHUVANSHI

Digitally signed by RAJEEV SINGH RAGHUVANSHI
DN: c=IN, o=CENTRAL DRUGS STANDARD
CONTROL ORGANIZATION, ou=RAJEEV SINGH
RAGHUVANSHI,
2.5.4.20=80c626a23e4eafbe8a239774cdeb03c27
69041015a06564fe67f54b765db1cb,
postalCode=600034, st=TAMIL NADU,
serialNumber=657F5E47D940985D8F03BDC902D
0E1FE73CFA12A1A126EA94FA5701124A19013,
cn=RAJEEV SINGH RAGHUVANSHI
Date: 2023.11.28 14:36:00 +05'30'

4	Generic Name:X-Ray Machine Radiography (Mobile) HF Model No.:STARNUKE-HF100 - Diagnostic X-ray machine Mobile type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 100 kVp Output power 5 KW ,SMART PRIMA X - Diagnostic X-ray machine Mobile type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 110 kVp Output power 5 KW , XRAYINDIA HF100 - Diagnostic X-ray machine Mobile type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 100 kVp Output power 5 KW ,STARNUKE-HF100 Mobile Digital Radiography System - Diagnostic Digital Radiography System Mobile type High frequency generator For rated line voltage 230V frequency 50Hz Single phase Output Current 100mA Peak Output Voltage 100kVp Output power 5KW ,SMART PRIMA X Mobile Digital Radiography System - Diagnostic Digital Radiography System Mobile type High frequency generator For rated line voltage 230V frequency 50Hz Single phase Output Current 100mA Peak Output Voltage 110kVp Output power 5KW ,XRAYINDIA HF100 Mobile Digital Radiography System - Diagnostic Digital Radiography System Mobile type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 100 kVp Output power 5 KW Intended Use:It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. Class of medical device:Class C Material of construction:Metal Body Dimension(if any): Shelflife:15 Years Sterile or Non sterile:Non-Sterilized Brand Name(if registered under the Trade Marks Act, 1999):STARNUKE
---	--

**RAJEEV SINGH
RAGHUVANSH**

Digitally signed by RAJEEV SINGH RAGHUVANSHI
DN: c=IN, o=CENTRAL DRUGS STANDARD
CONTROL ORGANIZATION, ou=RAJEEV SINGH
RAGHUVANSHI,
2.5.4.20=80c62f6a23e4eafbe8a239774cdeb03c276
9041015a06564fec7f54b765db1c5,
postalCode=600034, st=TAMIL NADU,
serialNumber=657F5E47D940985D8F038DC902D0
E1FE73CFA12A1A126EA9FA5701124A19013,
cn=RAJEEV SINGH RAGHUVANSHI
Date: 2023.11.28 14:36:12 +05'30'

5	Generic Name:X-Ray Machine Radiography (Mobile) LF Model No.:STARNUKE-MX100 - Diagnostic Mobile X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,XRAYINDIA 100M - Diagnostic Mobile X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW , RadX-100M - Diagnostic Mobile X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,STARNUKE-MX100 Mobile Digital Radiography System - Diagnostic Mobile Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,XRAYINDIA 100M Mobile Digital Radiography System - Diagnostic Mobile Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,RadX-100M Mobile Digital Radiography System - Diagnostic Mobile Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW Intended Use:It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. Class of medical device:Class C Material of construction:Metal Body Dimension(if any): Shelflife:15 Years Sterile or Non sterile:Non-Sterilized Brand Name(if registered under the Trade Marks Act, 1999):STARNUKE
---	--

RAJEEV SINGH
RAGHUVANSHI
HI

Digitally signed by RAJEEV SINGH RAGHUVANSHI
DN: cn=RAJEEV SINGH RAGHUVANSHI, ou=RAJEEV SINGH RAGHUVANSHI, 2.5.4.20=80c62f6a23e4eafbe8a239774cdeb03c2769041015a06564fe67f54b765db1cb, postalCode=600034, st=TAMIL NADU, serialNumber=657F5E47D940985D8F03BDC902D0E1FE73CFA12A1A126EA94FA5701124A19013, cn=RAJEEV SINGH RAGHUVANSHI
Date: 2023.11.28 14:36:32 +05'30'

6	Generic Name:X-Ray Machine Radiography (Fixed) LF Model No.:STARNUKE-FX100 - Diagnostic Fixed X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Peak Output Voltage 100kVp output power 8kW with Table ,STARNUKE-FX300 - Diagnostic X-ray machine Permanently Installed type Six Pulse Line Frequency Generator For rated line voltage 230 ± 10 V frequency 50 Hz Three phase Current 300 mA Rated Peak Output Voltage 125 kVp Output power 24 kW with Table ,XRAYINDIA 100F - Diagnostic Fixed X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table ,RadX-100F - Diagnostic Fixed X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table ,STARNUKE-FX100 Digital Radiography System - Diagnostic Fixed Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table ,STARNUKE-FX300 Digital Radiography System - Diagnostic Fixed Digital Radiography System Permanently Installed type Six Pulse Line Frequency Generator For rated line voltage 230 ± 10 V frequency 50 Hz Three phase Current 300 mA Rated Peak Output Voltage 125 kVp Output power 24 kW with Table ,XRAYINDIA 100F Digital Radiography System - Diagnostic Fixed Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table ,RadX-100F Digital Radiography System - Diagnostic Fixed Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table Intended Use:It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. Class of medical device:Class C Material of construction:Metal Body Dimension(if any): Shelflife:15 Years Sterile or Non sterile:Non-Sterilized Brand Name(if registered under the Trade Marks Act, 1999):STARNUKE
---	---

Digitally signed by RAJEEV SINGH RAGHUVANSHI
 DN: cn=RAJEEV SINGH RAGHUVANSHI, o=CENTRAL LICENSING AUTHORITY
 CONTROL ORGANIZATION, ou=RAJEEV SINGH RAGHUVANSHI
 2.5.4.20=80x326a23e4aafbe8a239774cdeb03c276
 9041015a06564fe67f54b765db1cb,
 postalCode=600034, st=TAMIL NADU,
 serialNumber=657F5E47D940985D8F038DC902D0
 E1FE73CFA12A1A126EA94FA5701124A19013,
 cn=RAJEEV SINGH RAGHUVANSHI
 Date: 2023.11.28 14:36:43 +05'30'

Place:

Date28-Nov-23

Central Licensing Authority



Directorate General of Health Services
Central Drugs Standard Control Organisation

Ministry of Health and Family Welfare
(Medical Device and Diagnostic Division)

File No : **MD/PostAppr/2024/27838**

FDA Bhawan, Kotla Road
New Delhi-110002
Phone No-011-23236965
Fax: 23236973
Date: 29-Jan-2025

To

M/s STAR NUKE CONSULTING ENGINEERING SERVICES
PRIVATE LIMITED, PLOT NO. 25, NAVKAR NAGAR,
KALYANPURA, NEW SANGANER ROAD, SANGANER SANGANER,
Jaipur, Rajasthan (India) - 302020 Telephone No.: 1416764685 FAX:
1416764685 Email: BSRAJORA@GMAIL.COM

Sub: Post approval change in Manufacturing License No. **MFG/MD/2023/001000** Dated **28/11/2023** .

Sir,

This is with reference to your application number **MD/PostAppr/2024/27838** dated **29/01/2025** regarding the above subject.

The Change in Manufacturing Licence No. **MFG/MD/2023/001000** as mentioned below is approved with subject to the same condition of licence.

Change Description	Product Name(Brand Name)	In Place of	To be Read as
Amendment/Correction/Others	X-Ray Machine Radiography (Fixed) HF (STARNUKE), Dental Handheld X-Ray Machine HF (STARNUKE), X-Ray Machine Radiography (Portable) HF (STARNUKE), X-Ray Machine Radiography (Mobile) HF(STARNUKE), X-Ray Machine Radiography (Mobile) LF(STARNUKE), X-Ray Machine Radiography (Fixed) LF(STARNUKE)	All Models are approved as per application form MD-7 but accessories were missing in License. So post approval change was applied and we got approval mentioning RVG and Wired DR System as accessory against application number MD/PostAppr/2024/21862 dated 11/09/2024.	Wireless DR System as accessory was not mentioned in application number MD/PostAppr/2024/21862 dated 11/09/2024. Same has been emailed to startupinnov@cdsco.nic.in dated 18-09-2024 for [Correction under category "Amendment/Corrections/ Others" - Addition of Accessory - Wireless DR System]

RAJEEV SINGH
RAGHUVANSHI

Digitally signed by RAJEEV SINGH RAGHUVANSHI
DN: c=IN, o=CENTRAL DRUGS STANDARD CONTROL
ORGANISATION, ou=CENTRAL DRUGS STANDARD
CONTROL ORGANISATION,
2.5.4.20=42d7189b1c0981bb5a263a4a73d025ff4b11b680a
91f08773480400a43ee361b, postalCode=110002, st=Delhi,
serialNumber=657f5e47d940985d8f03bdc902d0e1fc73cfa1
2a1a126ea94fa5701124a19013, cn=RAJEEV SINGH
RAGHUVANSHI
Date: 2025.01.29 16:09:53 +05'30'

LICENSING AUTHORITY



Directorate General of Health Services
Central Drugs Standard Control Organisation

Ministry of Health and Family Welfare
(Medical Device and Diagnostic Division)

File No : MD/PostAppr/2024/21862

FDA Bhawan, Kotla Road
New Delhi-110002
Phone No-011-23236965
Fax: 23236973
Date: 11-Sep-2024

To

M/s STAR NUKE CONSULTING ENGINEERING SERVICES
PRIVATE LIMITED, PLOT NO. 25, NAVKAR NAGAR,
KALYANPURA, NEW SANGANER ROAD, SANGANER SANGANER,
Jaipur, Rajasthan (India) - 302020 Telephone No.: 1416764685 FAX:
1416764685 Email: BSRAJORA@GMAIL.COM

Sub: Post approval change in Manufacturing License No. MFG/MD/2023/001000 Dated 28/11/2023 .

Sir,

This is with reference to your application number MD/PostAppr/2024/21862 dated 11/09/2024 regarding the above subject.

The Change in Manufacturing Licence No. MFG/MD/2023/001000 as mentioned below is approved with subject to the same condition of licence.

Change Description	Product Name(Brand Name)	In Place of	To be Read as
Amendment/Correction/Others	X-Ray Machine Radiography (Fixed) HF (STARNUKE), Dental Handheld X-Ray Machine HF (STARNUKE), X-Ray Machine Radiography (Portable) HF (STARNUKE), X-Ray Machine Radiography (Mobile) HF(STARNUKE), X-Ray Machine Radiography (Mobile) LF(STARNUKE), X-Ray Machine Radiography (Fixed) LF(STARNUKE)	All Models are approved as per application form MD-7 but accessories are missing in License	Addition of accessories RVG Sensor and Wired DR System in the approved devices

RAJEEV SINGH
RAGHUVANSHI
LICENSING AUTHORITY

Digitally signed by RAJEEV SINGH RAGHUVANSHI
DN: cn=IN, o=CENTRAL DRUGS STANDARD CONTROL
ORGANISATION, ou=CENTRAL DRUGS STANDARD CONTROL
ORGANISATION,
2.5.4.20=42d7189b1c0981bb5a263a4a73d025ff4b11b680a91f
08773480400a43ee361b, postalCode=110002, st=Delhi,
serialNumber=657f5e47d940985d8f03bdc902d0e1fe73cfa12a
Date: 2024.09.12 12:14:31 +05'30'

**Government of India
Directorate General of Health Services
Central Drugs Standard Control Organisation
Ministry of Health and Family Welfare
(Medical Device and Diagnostic Division)**

Food & Drugs Administration Bhawan
Kotla Road, New Delhi-110002
Date : 18/03/2025

To,

M/S. STAR NUKE CONSULTING ENGINEERING
SERVICES PRIVATE LIMITED
Plot No 25, Navkar Nagar ,Jaipur Rajasthan ,
302020,1416764685, 9950041555, India

Subject: Issuance of Non Conviction Certificate for Medical Devices.

Sir,

This is with reference to your file no **NCC/MD/2025/148920** dated **04-MAR-2025** for Issuance of Non conviction Certificate for Medical Devices approved in the manufacturing/import license.

The Non Conviction Certificate **NCC/MD/2025/000290** with respect to medical devices approved under manufacturing/import license no. **MFG/MD/2023/001000** dated : **28-NOV-2023** is enclosed herewith.

Date : 18/03/2025

**RAJEEV SINGH
RAGHUVANSHI**

Digitally signed by RAJEEV SINGH RAGHUVANSHI
DN: c=IN, o=CENTRAL DRUGS STANDARD CONTROL
ORGANISATION, ou=CENTRAL DRUGS STANDARD CONTROL
ORGANISATION,
2.5.4.20=42d7189b1c0981bb5a263a4a73d025ff4b11b680a9
1b08773480400a43ee361b, postalCode=110002, st=Delhi,
serialNumber=657f5e47d940985d8f03bdc902d0e1fe73cfa1
2a1a726ea9f4a5701124a19013, cn=RAJEEV SINGH
RAGHUVANSHI
Date: 2025.03.18 15:01:25 +05'30'

Competent Authority

CERTIFICATE



No. 0P250304.SNCU083

Test Report / Technical Construction File no. TLHK25022867452 TEHK25022867453

Certificate's
Holder:

STAR NUKE CONSULTING ENGINEERING SERVICES
PRIVATE LIMITED

Plot no. 27, Radha Nikunj-B, Iskcon Road, Near Hotel Hayatt
Regency, Kharbas Circle, Mansarovar, Jaipur, Rajasthan,
302020, India.

Certification
ECM Mark



Product:

Flat Panel detector (Wired and Wireless)

Model(s):

STARNUKE4343DI, STARNUKE4343DIW, STARNUKE3543DI,
STARNUKE3543DIW

Verification to:

Standard:

EN 61010-1:2010+A1:2019, EN IEC 61326-1:2021

related to CE Directive(s):

2014/35/EU (Low Voltage)

2014/30/EU (Electromagnetic Compatibility)

Remark:

The manufacturer has voluntarily decided to submit its documents concerning the above-mentioned product for verification. Ente Certificazione Macchine confirms that the documentation made available and immediately returned to it, as containing sensitive data, meets the essential requirements of the above-mentioned directive/standard. The verification activity carried out exclusively concerned the technical documentation and no verification was carried out on the product. This document cannot replace the EC Declaration of Conformity. This document was issued in accordance with regulation RGVOL01 published on the website of www.entecerma.it and concerning voluntary certifications with a non-notified procedure.

Issuance date: 04 March 2025

Expiry date: 03 March 2030

For online check:



Approver

Ente Certificazione Macchine
Legal Representative
Luca Bedonni



TEST REPORT AS PER: IS/IEC 60529: 2001 (Reaffirmed Year: 2019)
IP68 as per IS/IEC 60529: 2001 (Reaffirmed Year: 2019)

Name & Address of Customer: STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED Plot No. 25, Navkar Nagar, New Sanganer Road, Kalyanpura, Sanganer, Jaipur, Rajasthan, 302020	Test Report No: ATLTR20240921-013		Date of issue: 24-09-2024	
	Discipline: Electrical		Group: Environmental Test Facility	
	ULR-TC877824000000771F			
	Date of Sample Receipt: 21/09/2024		Start of Test Date: 23/09/2024	
				End of Test Date: 24/09/2024

PART A - PARTICULARS OF THE SAMPLE SUBMITTED

Sample description	Product Name: Digital Radiography System (DR) Model Name: STARNUKE4343DIW
Grade/ variety/ type/ class/ size etc.	Input Rating: 18Vdc, 3.5A
Declared values, if any	IP68 as per IS/IEC 60529 : 2001 (Reaffirmed Year : 2019)
Batch No., Date of Manufacture and Brand Name	Brand / Trademark: "STAR NUKE"
Quantity	1 No.
Condition of the sample	Good Condition
Environmental conditions	Temperature : 15°C to 35°C Relative humidity : 25 % to 75%
Location	Permanently
Remark	--

PART B - SUPPLEMENTARY INFORMATION

- a) Deviations from the test methods as per relevant specification/ standard operating procedure, if any: Nil.
b) Details of the drawings, graphs, tables, sketches or Photographs as referred in the test report, if any: Nil.

Notes:

- i) This report is not to be reproduced wholly or in part without our special permission in writing.
ii) This report refers only to the particular sample detailed above.
iii) The results reported in this certificate are valid at the time of and under the stipulated conditions of measurement.


<u>Tested by</u>	<u>Reviewed & Approved by</u>	<u>Issued by</u>
RAHUL KUMAR Digitally signed by RAHUL KUMAR	MOHD AHMAD BAIG Digitally signed by MOHD AHMAD BAIG	MOHD AHMAD BAIG Digitally signed by MOHD AHMAD BAIG
<u>Rahul Kumar</u> (Testing Engineer)	<u>Mohd Ahmad Baig</u> (Technical Manager)	<u>Mohd Ahmad Baig</u> (Technical Manager)

PART C- TEST RESULTS

S. No.	Cl. No.	Test / Requirement	Test result / observation	Verdict
1	12	Tests for protection against access to hazardous parts indicated by the first characteristic numeral.	See below	P
	12.2	Test conditions for first characteristic numerals 6.	See below	P
		The access probe of 1,0mm Ø shall not penetrate	Complies	P
	12.3	Acceptance conditions for first characteristic numerals 6.	See below	P
		The protection is satisfactory if adequate clearance is kept between the access probe and hazardous parts.	Complies	P
2	13	Tests for protection against solid foreign objects indicated by the first characteristic numeral	See below	P
	13.4	Dust test for first characteristic numerals 6	See below	P
		The talcum powder used shall be able to pass through a square-meshed sieve the nominal wire diameter of which is 50µm and the nominal width of a gap between wires 75 µm. The amount of talcum powder to be used is 2 kg per cubic meter of the test chamber volume.	Complies	P
	13.6	Acceptance conditions for first characteristic numerals 6.	See below	P
		The protection is satisfactory if no deposition of dust is observable inside the enclosure at the end of the test.	No deposition of dust observed inside the enclosure.	P

S. No.	Cl. No.	Test / Requirement	Test result/ observation	Verdict
3	14	Test for protection against water indicated by the second characteristic numeral	See below	P
	14.2.8	Test conditions for Second characteristic numerals 8	See below	P
		The test is made by completely immersing the enclosure in water in its service position so that the following conditions are satisfied:	Complies	P
		The lowest point of enclosures is located 2000mm below the surface of the water for 2 hour.	Complies	P
		The water temperature does not differ from that of the equipment by more than 5K.	Complies	P
	14.3	Acceptance conditions for second characteristic numerals 8	See below	P
		Enclosure inspected for ingress of water	No ingress of water observed inside the enclosure	P
		In general, if any water has entered, it shall not:	See above	N/A
		- be sufficient to interfere with the correct operation of the equipment or impair safety	See above	N/A
		- deposit on insulation parts where it could lead to tracking along the creepage distances	See above	N/A
		- reach live parts or windings not designed to operate when wet	See above	N/A
		- accumulate near the cable end or enter the cable if any	See above	N/A

Pictorial View Of The Equipment

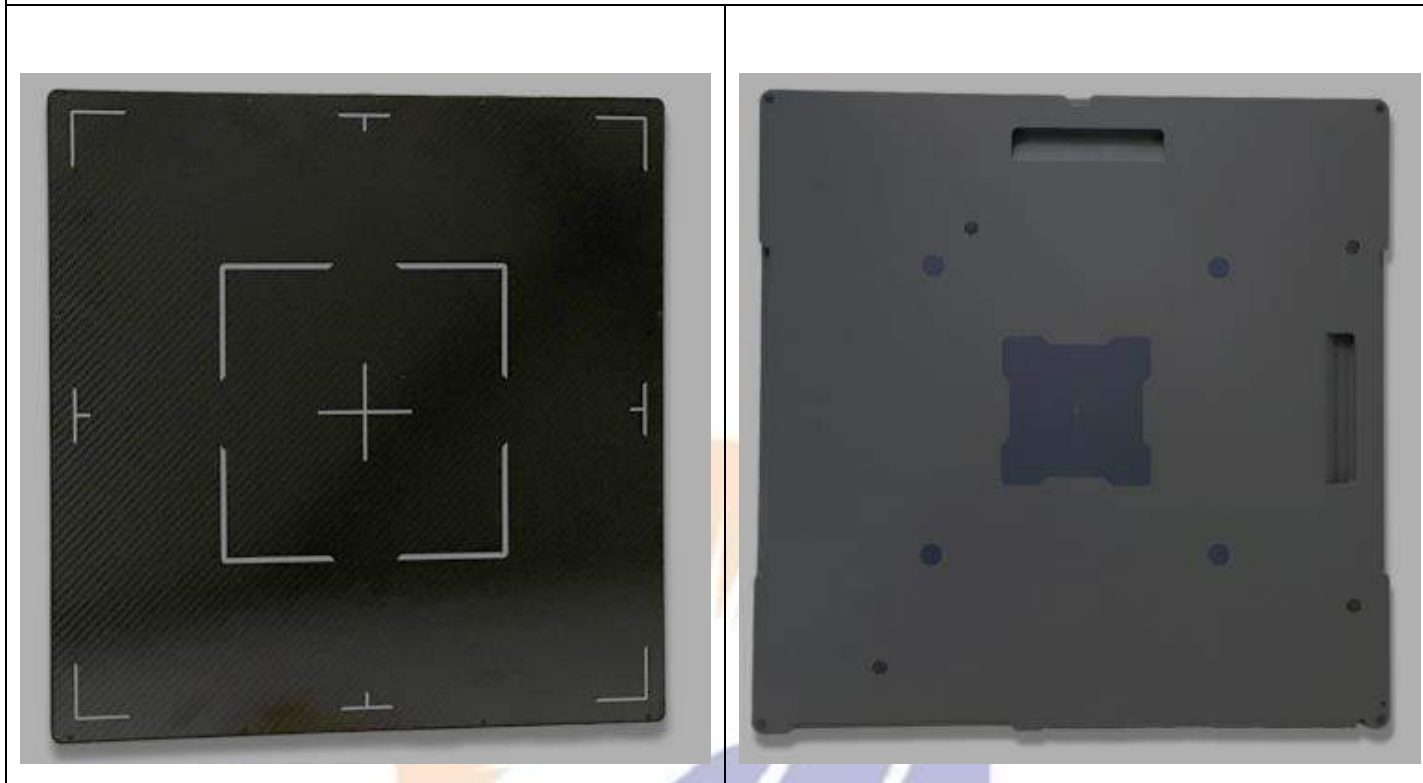

Abbreviations: - 1. P = PASS.
2. F = FAIL.
3. N/A = NOT APPLICABLE.
4. --- = No compliance required

Conclusion: Sample complies with IP68 requirements as per IS/IEC 60529: 2001 (RA 2019).

<u>Tested by</u>	<u>Reviewed & Approved by</u>	<u>Issued by</u>
RAHUL KUMAR Digitally signed by RAHUL KUMAR	MOHD AHMAD BAIG Digitally signed by MOHD AHMAD BAIG	MOHD AHMAD BAIG Digitally signed by MOHD AHMAD BAIG
<u>Rahul Kumar</u> (Testing Engineer)	<u>Mohd Ahmad Baig</u> (Technical Manager)	<u>Mohd Ahmad Baig</u> (Technical Manager)

---END OF TEST REPORT---



Certificate of Registration

This is to certify that

STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED

**PLOT NO. 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD,
SANGANER, JAIPUR - 302020, RAJASTHAN, INDIA.**

has been independently assessed by QRO
and is compliant with the requirement of:

ISO 13485:2016

Quality Management System for Medical Devices

For the following scope of activities:

- MANUFACTURING AND SUPPLY OF DIAGNOSTIC RADIOLOGY X RAY EQUIPMENT
1. DIGITAL RADIOGRAPHY PANEL (FLAT PANEL DETECTOR - WIRED AND WIRELESS)
 2. MOBILE AND FIXED X RAY RADIOGRAPHY MACHINE
 3. MOBILE AND FIXED DIGITAL RADIOGRAPHY MACHINE (X RAY SOURCE WITH DIGITAL IMAGING PANEL)
 4. ULTRA PORTABLE HANDHELD X RAY MACHINE
 5. HANDHELD DENTAL X RAY MACHINE
 6. DENTAL IOP R-DENT X RAY MACHINE
 7. RVG (RADIOVISIOGRAPHY) DENTAL IMAGING SENSOR AND ITS ACCESSORIES
 8. C- ARM, RADIOGRAPHIC AND FLUOROSCOPIC X RAY SYSTEM
 9. PORTABLE X RAY MACHINE

Date of Certification: 28th February 2025

1st Surveillance Audit Due: 27th February 2026

2nd Surveillance Audit Due: 27th February 2027

Certificate Expiry: 27th February 2028

Certificate Number: 305025022818MD




Head of Certification

Validity of this certificate is subject to annual surveillance audits to be done successfully on or before 365 days from date of the audit.
(In case surveillance audit is not allowed to be conducted; this certificate shall be suspended / withdrawn).

The Validity of this certificate can be verified at www.qrocert.org

This certificate of registration remains the property of QRO Certification LLP and shall be returned immediately upon request.

India Office : QRO Certification LLP

142, 11nd Floor, Avtar Enclave, Near Paschim Vihar West Metro Station, Delhi-110063, (INDIA)

Website : www.qrocert.org, E-mail : info@qrocert.org

Certificate of Registration



This is to Certify That The Quality Management System of

STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED

PLOT NO. 25, NAVKAR NAGAR, NEW SANGANER ROAD, KALYANPURA, SANGANER,
JAIPUR - 302020, RAJASTHAN, INDIA.

has been assessed and found to conform to the requirements of

ISO 9001:2015

for the following scope :

1. MANUFACTURING AND SUPPLY OF DIAGNOSTIC RADIOLOGY X RAY EQUIPMENT: X RAY IMAGING SYSTEM, MOBILE AND FIXED X RAY RADIOGRAPHY SYSTEM (LINE AND HIGH FREQUENCY), HAND-HELD PORTABLE X RAY SYSTEM (LINE AND HIGH FREQUENCY), HAND-HELD HIGH FREQUENCY DENTAL X RAY SYSTEM, DENTAL IOP LINE FREQUENCY X RAY SYSTEM, C- ARM, RADIOGRAPHIC AND FLUOROSCOPIC X RAY SYSTEM (LINE AND HIGH FREQUENCY).
2. MANUFACTURING AND SUPPLY OF X RAY BASED INSPECTION SYSTEM: X RAY DIFFRACTOMETER, X RAY FLUORESCENCE DEVICE (HAND-HELD & CABINET TYPE), BAGGAGE INSPECTION SYSTEM, PORTABLE SCANNERS, FOOD INSPECTION SYSTEM, PCB ANALYZERS, FILL LEVEL INSPECTION SYSTEM.
3. MANUFACTURING AND SUPPLY OF RADIATION SAFETY PERSONNEL PROTECTIVE EQUIPMENT (LEAD APRON, LEAD HAND GLOVES, LEAD HEAD CAP, LEAD GONAD SHIELD, LEAD THYROID COLLAR, LEAD FREE APRON, LEAD BARRIER, LEAD GOGGLES, LEAD VEST SKIRT)
4. SUPPLY OF INDUSTRIAL OCCUPATIONAL AND BREATHING APPARATUS, HELMET, SAFETY GOGGLES, RUBBER HAND GLOVES, HALF AND FULL-FACE GAS MASK.
5. SALES OF X RAY BASED METAL DETECTOR AND RADIATION DOSE MONITORING EQUIPMENT.
6. PROVIDING QUALITY ASSURANCE TESTING SERVICE AS PER AERB & NABL COMPLIANCE FOR DIAGNOSTIC RADIOLOGY EQUIPMENT.
7. PROVIDING CONSULTANCY AND PROJECT MANAGEMENT SERVICES FOR AERB REGULATORY COMPLIANCE FOR INDUSTRIAL AND MEDICAL X RAY / GAMMA BASED RADIATION PROCESSING FACILITIES.

Certificate No

23DQMJO6

Initial Registration Date : 01/11/2023

Issuance Date : 01/11/2023

Date of Expiry* : 31/10/2026

1st Surve. Due : 01/10/2024

2nd Surve. Due : 01/10/2025



DIRECTOR

ROHS Certification Pvt. Ltd.

B-7, 1st Floor, Sector-2 Noida, Gautam Budh Nagar, UP-201301

e-mail : info@rohscertification.co.in | website : www.rohscertification.co.in

The Registration is not a Product Quality Certificate. *Subject to successful completion of surveillance audits, Visit for verification on www.rohscertification.co.in
Certificate is the property of ROHS and return when demanded



CB-QMS-035

Certificate of Compliance



This is to Certify that The Quality Management Customer Satisfaction System of

**STAR NUKE CONSULTING ENGINEERING SERVICES
PRIVATE LIMITED**

PLOT NO. 25, NAVKAR NAGAR, NEW SANGANER ROAD, KALYANPURA, SANGANER,
JAIPUR - 302020, RAJASTHAN, INDIA.

has been assessed and found to conform to the requirements of

ISO 10002:2018

for the following scope :

1. MANUFACTURING AND SUPPLY OF DIAGNOSTIC RADIOLOGY X RAY EQUIPMENT: X RAY IMAGING SYSTEM, MOBILE AND FIXED X RAY RADIOGRAPHY SYSTEM (LINE AND HIGH FREQUENCY), HAND-HELD PORTABLE X RAY SYSTEM (LINE AND HIGH FREQUENCY), HAND-HELD HIGH FREQUENCY DENTAL X RAY SYSTEM, DENTAL IOP LINE FREQUENCY X RAY SYSTEM, C- ARM, RADIOGRAPHIC AND FLUOROSCOPIC X RAY SYSTEM (LINE AND HIGH FREQUENCY).
2. MANUFACTURING AND SUPPLY OF X RAY BASED INSPECTION SYSTEM: X RAY DIFFRACTOMETER, X RAY FLUORESCENCE DEVICE (HAND-HELD & CABINET TYPE), BAGGAGE INSPECTION SYSTEM, PORTABLE SCANNERS, FOOD INSPECTION SYSTEM, PCB ANALYZERS, FILL LEVEL INSPECTION SYSTEM.
3. MANUFACTURING AND SUPPLY OF RADIATION SAFETY PERSONNEL PROTECTIVE EQUIPMENT (LEAD APRON, LEAD HAND GLOVES, LEAD HEAD CAP, LEAD GONAD SHIELD, LEAD THYROID COLLAR, LEAD FREE APRON, LEAD BARRIER, LEAD GOGGLES, LEAD VEST SKIRT)
4. SUPPLY OF INDUSTRIAL OCCUPATIONAL AND BREATHING APPARATUS, HELMET, SAFETY GOGGLES, RUBBER HAND GLOVES, HALF AND FULL-FACE GAS MASK.
5. SALES OF X RAY BASED METAL DETECTOR AND RADIATION DOSE MONITORING EQUIPMENT.
6. PROVIDING QUALITY ASSURANCE TESTING SERVICE AS PER AERB & NABL COMPLIANCE FOR DIAGNOSTIC RADIOLOGY EQUIPMENT.
7. PROVIDING CONSULTANCY AND PROJECT MANAGEMENT SERVICES FOR AERB REGULATORY COMPLIANCE FOR INDUSTRIAL AND MEDICAL X RAY / GAMMA BASED RADIATION PROCESSING FACILITIES.

Certificate No : **23DQMJ06**

Initial Registration Date : 01/11/2023

Date of Expiry* : 31/10/2026

1st Sur date : 01/10/2024

Issuance Date : 01/11/2023

2nd Sur Date : 01/10/2025

DIRECTOR
ROHS Certification Pvt. Ltd.

B-7, 1st Floor, Sector-2 Noida, Gautam Budh Nagar, UP-201301

e-mail : info@rohscertification.co.in | website : www.rohscertification.co.in

The Registration is not a Product Quality Certificate, *Subject to successful completion of surveillance audits, Visit for verification on www.rohscertification.co.in Certificate is the property of ROHS and return when demanded

Certificate of Registration



This is to Certify That
The Occupational Health & Safety Management System of
STAR NUKE CONSULTING ENGINEERING SERVICES
PRIVATE LIMITED

PLOT NO. 25, NAVKAR NAGAR, NEW SANGANER ROAD, KALYANPURA, SANGANER,
 JAIPUR - 302020, RAJASTHAN, INDIA.

has been assessed and found to conform to the requirements of

ISO 45001:2018

for the following scope :

1. MANUFACTURING AND SUPPLY OF DIAGNOSTIC RADIOLOGY X RAY EQUIPMENT: X RAY IMAGING SYSTEM, MOBILE AND FIXED X RAY RADIOGRAPHY SYSTEM (LINE AND HIGH FREQUENCY), HAND-HELD PORTABLE X RAY SYSTEM (LINE AND HIGH FREQUENCY), HAND-HELD HIGH FREQUENCY DENTAL X RAY SYSTEM, DENTAL IOP LINE FREQUENCY X RAY SYSTEM, C- ARM, RADIOGRAPHIC AND FLUOROSCOPIC X RAY SYSTEM (LINE AND HIGH FREQUENCY).
2. MANUFACTURING AND SUPPLY OF X RAY BASED INSPECTION SYSTEM: X RAY DIFFRACTOMETER, X RAY FLUORESCENCE DEVICE (HAND-HELD & CABINET TYPE), BAGGAGE INSPECTION SYSTEM, PORTABLE SCANNERS, FOOD INSPECTION SYSTEM, PCB ANALYZERS, FILL LEVEL INSPECTION SYSTEM.
3. MANUFACTURING AND SUPPLY OF RADIATION SAFETY PERSONNEL PROTECTIVE EQUIPMENT (LEAD APRON, LEAD HAND GLOVES, LEAD HEAD CAP, LEAD GONAD SHIELD, LEAD THYROID COLLAR, LEAD FREE APRON, LEAD BARRIER, LEAD GOGGLES, LEAD VEST SKIRT)
4. SUPPLY OF INDUSTRIAL OCCUPATIONAL AND BREATHING APPARATUS, HELMET, SAFETY GOGGLES, RUBBER HAND GLOVES, HALF AND FULL-FACE GAS MASK.
5. SALES OF X RAY BASED METAL DETECTOR AND RADIATION DOSE MONITORING EQUIPMENT.
6. PROVIDING QUALITY ASSURANCE TESTING SERVICE AS PER AERB & NABL COMPLIANCE FOR DIAGNOSTIC RADIOLOGY EQUIPMENT.
7. PROVIDING CONSULTANCY AND PROJECT MANAGEMENT SERVICES FOR AERB REGULATORY COMPLIANCE FOR INDUSTRIAL AND MEDICAL X RAY / GAMMA BASED RADIATION PROCESSING FACILITIES.

Certificate No

23DOMU07

Initial Registration Date : 01/11/2023

Issuance Date : 01/11/2023

Date of Expiry* : 31/10/2026

1st Surve. Due : 01/10/2024

2nd Surve. Due : 01/10/2025



DIRECTOR

ROHS Certification Pvt. Ltd.

B-7, 1st Floor, Sector-2 Noida, Gautam Budh Nagar, UP-201301

e-mail : info@rohscertification.co.in | website : www.rohscertification.co.in

The Registration is not a Product Quality Certificate, *Subject to successful completion of surveillance audits, Visit for verification on www.rohscertification.co.in
 Certificate is the property of ROHS and return when demanded





राष्ट्रीय लघु उद्योग निगम लिमिटेड THE NATIONAL SMALL INDUSTRIES CORPORATION LIMITED

(A Government of India Enterprise)

SNW/JAI/08/19755
189545

Branch Office : NF/0/2, NEHRU PLACE, TONK ROAD, JAIPUR-302015

Ph : 01412742991

Fax : 01412741277

Email : bojai@nsic.co.in Website : www.nsic.co.in



GOVERNMENT PURCHASE ENLISTMENT CERTIFICATE

(Valid From 04/08/2025 to 03/08/2027)

Ref.No NSIC/GP/JAI/2024/109680

Date: 11/08/2025

M/s. STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED

Plot No. 27, Radha Nikunj B, At 200 Feet Kharbas Circle, Mansarovar, near to Hotel Hayat, Jaipur, Rajasthan 302020
JAIPUR, RAJASTHAN- 302020

Factory Address:

1 .Plot No. 27, Radha Nikunj B, At 200 Feet Kharbas Circle, Mansarovar, near to Hotel Hayat, Jaipur, Rajasthan 302020
JAIPUR, RAJASTHAN -302020
2 .Services:Plot No. 27, Radha Nikunj B, At 200 Feet Kharbas Circle, Mansarovar, near to Hotel Hayat JAIPUR, RAJASTHAN -302020

Name of the Directors

1.BALRAM SINGH RAJORA

2.USHA RAO

Constitution: Private Limited

Udyam Registration Number UDYAM-RJ-17-0020564

Enterprise Social Class: GENERAL

Special Category: GENERAL

GOVERNMENT PURCHASE REGISTRATION NO: NSIC/GP/JAI/2025/0055906

Monetary Limit: ₹ 882 lakhs (₹ Eight Hundred Eighty Two Lakh Only)
TURNOVER (Rupees in Lakhs)

Financial Year	Annual Turnover
2021-22	119.2
2022-23	432.16
2023-24	1763.16
Monetary Limit	882

MSEs registered with NSIC are exempted from deposit of Earnest Money irrespective of value of Monetary Limit. Your name has been registered as a MSE Unit eligible for participation in the **Central Government Store Purchase Programme** as per the **Single Point Registration Scheme** for the following Item(s)/Store(s)/Service(s).

Name of the Store(s)/ Service(s)	Specification(s)	Qualitative Capacity	Quantitative Capacity P.M.
----------------------------------	------------------	----------------------	----------------------------

"As per List Attached" (9 item only)

Disclaimer:-1.The purchasing agencies are advised to satisfy themselves with the store details in the certificate while doing the Technical Evaluation stage before placing the tender/order on the units, certified by NSIC.

2. This certificate will be valid subject to compliance of definition (Composite criteria of investment and turnover for classification of Micro, Small Enterprises as per MSMED Act).



Mukeshgupta

M/s. STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED

Authorised Signatory



Authenticity of the certificate can be checked through the web portal: www.nsicsonline.com

CIN : U74140DL1955GOI002481

Conditions overleaf.



राष्ट्रीय लघु उद्योग निगम लिमिटेड THE NATIONAL SMALL INDUSTRIES CORPORATION LIMITED

(A Government of India Enterprise)

Sr. No. 286062

Branch Office : NF/0/2, NEHRU PLACE, TONK ROAD, JAIPUR-302015

Ph : 01412742991

Fax : 01412741277

Email : bojai@nsic.co.in Website : www.nsic.co.in



STORE DETAILS CERTIFICATE

(Valid From 04/08/2025 to 03/08/2027)

ANNEXURE TO GOVERNMENT PURCHASES ENLISTMENT CERTIFICATE

NO. NSIC/GP/JAI/2025/0055906 D.T. 11/08/2025

ISSUED TO M/s. STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED, RAJASTHAN

UNIT-1) Plot No 27, Radha Nikunj B, At 200 Feet Kharbas Circle, Mansarovar, near to Hotel Hayat, Jaipur, Rajasthan 302020, JAIPUR, RAJASTHAN-302020

Sno	Store(s)/ Service(s) Name	Specification(s)	Qualitative Capacity	Quantitative Capacity PM	Remarks
1	Ultra-Portable Handheld Diagnostic X Ray Machine NIC code: 2660	IS 7620 (PART-1): 1986 & AERB Type Approval & CDSCO Manufacturing License	Handheld Portable Type Attachment- With Tripod Generator: High Frequency -Tube Current: 2 mA to 10 mA - X Ray Beam Energy: 60 kV to 90 kV	50 Or	OEM
2	Medical Diagnostic X Ray Machine NIC code: 2660	IS 7620 (PART-1): 1986 & AERB Type Approval & CDSCO Manufacturing License	-Portable / Fixed / Mobile Type - Attachment- With wheel based Mobile Stand / Fixed Celling to Floor Mounted Stand With Horizontal Multi position; (Manual and Motorized) with Spot Film Device and Floating Tabletop Generator: Line Frequency: Tube Current- 10 mA to 500 mA & X-Ray Beam Energy- 40 kV to 125 kV High Frequency: Tube Current- 100 mA to 1000 mA / 3.5 kW to 80 kW & X-Ray Beam Energy- 40 kV to 150 kV	35 Or	OEM
3	C-Arm Fluoroscopy X Ray Machine NIC code: 2660	IS 7620 (PART-1): 1986 & AERB Type Approval & CDSCO Manufacturing License	High Frequency: Tube Current: 0.2 mA to 100 mA X Ray Beam Energy: 40 kV to 125 kV	2 Or	OEM
4	Dental X Ray Machine NIC code: 2660	IS 7620 (PART-1) 1986 & AERB Type Approval & CDSCO	Handheld / Floor Mounted / Wall Mounted Type Generator;	25 or	OEM

M/s. STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED



Mukesh Singh
Authorised Signatory

certificate can be checked through the web portal: www.nsicsonline.com

CIN : U74140DL1955GOI002481



राष्ट्रीय लघु उद्योग निगम लिमिटेड THE NATIONAL SMALL INDUSTRIES CORPORATION LIMITED

(A Government of India Enterprise)

Sr. No. 220003

Branch Office : NF/0/2, NEHRU PLACE, TONK ROAD, JAIPUR-302015

Ph : 01412742991

Fax : 01412741277

Email : bojai@nsic.co.in Website : www.nsic.co.in



STORE DETAILS CERTIFICATE

		Manufacturing License	Line Frequency: Tube Current- 08 mA to 10 mA & X-Ray Beam Energy- 60 kV to 70 kV High Frequency: Tube Current- 2 mA to 10 mA & X-Ray Beam Energy- 60 kV to 70 kV		
5	Digital Radiography System NIC code: 2660	IS 7620 (PART-1): 1986 & AERB Type Approval & CDSCO Manufacturing License	- Fixed / Mobile Type - Attachment- With wheel based Mobile Stand / Fixed Ceiling to Floor Mounted Stand With Horizontal Multi position; (Manual and Motorized) with Spot Film Device and Floating Tabletop Generator: Line Frequency: Tube Current- 10 mA to 500 mA & X-Ray Beam Energy- 40 kV to 125 kV High Frequency: Tube Current- 100 mA to 1000 mA / 3.5 kW to 80 kW & X-Ray Beam Energy- 40 kV to 150 kV	5 Or	OEM
6	DR Panel system NIC code: 2660	CE & CDSCO	Digital Radiography (DR) Panel / Flat Panel Detector for X Ray Size: 14 Inch X 17 Inch & 17 Inch X 17 Inch Attachment: Detector Protection Cover	25 Or	OEM
7	Dental Radiography (RVG) System NIC code: 2660	CDSCO	Dental X Ray Imaging sensor (RVG)	50 Or	OEM
8	Medical X Ray Imaging Film NIC code: 2023	ISO 13485	Medical X Ray imaging films sizes: A4, Minimum: 8 Inch x10 Inch to Maximum: 17 Inch x 17 Inch	1000	OEM

UNIT-2) Services: Plot No 27, Radha Nikunj B, At 200 Feet Kharbas Circle, Mansarovar, near to Hotel Hayat , JAIPUR, RAJASTHAN-302020

Sno	Name of Service/ Activities	Definition of Activity/ Service(s)	Quantitative Capacity/Services PM
1	Quality Assurance Testing of Medical & Dental X Ray Equipment NIC code: 7490	Quality Assurance Testing of Medical & Dental X Ray Equipment as per AERB & NABL.	Total Cumulative Capacity of 30 Nos.



Authorised Signatory

M/s. ST. NIKE ENGINEERING SERVICES PRIVATE LIMITED

Authorised Signatory

Certificate can be checked through the web portal: www.nsicsonline.com

CIN : U74140DL1955GOI002481



राष्ट्रीय लघु उद्योग निगम लिमिटेड
THE NATIONAL SMALL INDUSTRIES CORPORATION LIMITED
(A Government of India Enterprise)

Sr.No. JAI-20017334

Branch Office : NF/0/2, NEHRU PLACE, TONK ROAD, JAIPUR-302015

Ph : 01412742991

Fax : 01412741277

Email : bojai@nsic.co.in Website : www.nsic.co.in



STORE DETAILS CERTIFICATE

AGRA

Comments / Note

(Optional):MSME PPDC INSPECTION REPORT NO. PPDC/NSIC/Inspection/2025-26/65 Dated 14.07.2025

M/s. STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED

"Authenticity of the certificate can be checked through the web portal: www.nsiconline.com"



Authorised Signatory

[Handwritten Signature]



CIN : U74140DL1955GOI002481

Government of India
Directorate General of Health Services
Central Drugs Standard Control Organisation
Ministry of Health and Family welfare
(Medical Device and Diagnostic Division)
Market Standing Certificate

Certificate Number : MSC/MD/2025/000909

Dated : 03/10/2025

This is to certify that M/s. **STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED** situated at address **Plot No 25, Navkar Nagar ,Jaipur Rajasthan ,302020,1416764685, 9950041555, India Jaipur Rajasthan 302020 1416764685, 9950041555 India** is holding Manufacturing/Import License no. **MFG/MD/2023/001000** issued on **28-NOV-2023** Under this license, the said firm is permitted to manufacture/import of medical devices as stated in manufacturing/import license.

Name of the products with their product name and dimensions if any mentioned below :

S.NO	Medical Device Details
1	1. Generic Name :Dental Handheld X-Ray Machine HF 2. Brand Name :STARNUKE 3. Notified Category : X-Ray Machine 4. Class of Medical Device :Class C 5. Shelf life :15 Years 6. Sterile/Non-Sterile:Non-Sterilized 7. Intended Use :The use of Dental X-Ray Machine is to detect oral health issues, like cavities and gum disease, before they worsen. 8. Material of Construction: Fiber Plastic 9. Dimension: NA 10. Model/Catalogue No./Name :Ai Ray - Diagnostic X-ray machine Portable Handheld Dental For rated line voltage 240 V frequency 50 Hz Single Phase Current 2.5 mA Rated Peak voltage 65 kVp Output Power 162.5 W High Frequency Generator ,V-Light Eco - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 60 kV Output Power 120 W High Frequency Generator ,STARNUKE-DNTX - Diagnostic X-ray machine Portable Handheld Dental For rated line voltage 240 V frequency 50 Hz Single Phase Current 2.5 mA Rated Peak voltage 65 kVp Output Power 162.5 W High Frequency Generator ,Mini Ray - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator ,Ai-Ray - Diagnostic X-ray machine- Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 3 mA Rated Peak voltage 70 kV Output Power 210 W High Frequency Generator ,Waldent V-Light Eco - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 60 kV Output Power 120 W High Frequency Generator ,i-lite - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator ,Starlite Eco - Diagnostic X-ray machine Portable Handheld Battery Operated Dental X Ray Machine for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 60 kV Output Power 120 W High Frequency Generator

2	1. Generic Name :X-Ray Machine Radiography (Fixed) HF 2. Brand Name :STARNUKE 3. Notified Category : X-Ray Machine 4. Class of Medical Device :Class C 5. Shelf life :15 Years 6. Sterile/Non-Sterile:Non-Sterilized 7. Intended Use :It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. 8. Material of Construction: Metal Body 9. Dimension: NA 10. Model/Catalogue No./Name :STARNUKE-HF100R - Diagnostic X-ray machine Fixed type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100mA Rated Peak Output Voltage 110kVp Output power 5KW with Table , STARNUKE-HF300 - Diagnostic X-ray machine Stationary type High frequency generator For rated line voltage 230 V frequency 50 Hz three phase Output Current 320 mA Rated Peak Output Voltage 125 kVp Output power 20 KW with Table , STARNUKE-HF100R Digital Radiography System - Diagnostic Digital Radiography System Stationary type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 110 kVp Output power 5 KW with Table , STARNUKE-HF300 Digital Radiography System - Diagnostic Digital Radiography System Stationary type High frequency generator For rated line voltage 230 V frequency 50 Hz three phase Output Current 320 mA Rated Peak Output Voltage 125 kVp Output power 20 KW with Table
3	1. Generic Name :X-Ray Machine Radiography (Portable) HF 2. Brand Name :STARNUKE 3. Notified Category : X-Ray Machine 4. Class of Medical Device :Class C 5. Shelf life :15 Years 6. Sterile/Non-Sterile:Non-Sterilized 7. Intended Use :It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. 8. Material of Construction: Metal Body 9. Dimension: NA 10. Model/Catalogue No./Name :MINE 2IN - Diagnostic X-ray machine Portable Handheld Battery Operated for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator ,MIN-X - Diagnostic X-ray machine Portable Handheld Battery Operated for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator ,MIN-X Portable Digital Radiography System - Diagnostic Digital Radiography System Portable Handheld Battery Operated for rated line voltage 240 V 50 Hz Single Phase Current 2 mA Rated Peak voltage 70 kV Output Power 140 W High Frequency Generator

4	1. Generic Name :X-Ray Machine Radiography (Mobile) HF 2. Brand Name :STARNUKE 3. Notified Category : X-Ray Machine 4. Class of Medical Device :Class C 5. Shelf life :15 Years 6. Sterile/Non-Sterile:Non-Sterilized 7. Intended Use :It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. 8. Material of Construction: Metal Body 9. Dimension: NA 10. Model/Catalogue No./Name :STARNUKE-HF100 - Diagnostic X-ray machine Mobile type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 100 kVp Output power 5 KW ,SMART PRIMA X - Diagnostic X-ray machine Mobile type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 110 kVp Output power 5 KW ,XRAYINDIA HF100 - Diagnostic X-ray machine Mobile type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 100 kVp Output power 5 KW , STARNUKE-HF100 Mobile Digital Radiography System - Diagnostic Digital Radiography System Mobile type High frequency generator For rated line voltage 230V frequency 50Hz Single phase Output Current 100mA Peak Output Voltage 100kVp Output power 5KW , SMART PRIMA X Mobile Digital Radiography System - Diagnostic Digital Radiography System Mobile type High frequency generator For rated line voltage 230V frequency 50Hz Single phase Output Current 100mA Peak Output Voltage 110kVp Output power 5KW , XRAYINDIA HF100 Mobile Digital Radiography System - Diagnostic Digital Radiography System Mobile type High frequency generator For rated line voltage 230 V frequency 50 Hz Single phase Output Current 100 mA Rated Peak Output Voltage 100 kVp Output power 5 KW
5	1. Generic Name :X-Ray Machine Radiography (Mobile) LF 2. Brand Name :STARNUKE 3. Notified Category : X-Ray Machine 4. Class of Medical Device :Class C 5. Shelf life :15 Years 6. Sterile/Non-Sterile:Non-Sterilized 7. Intended Use :It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. 8. Material of Construction: Metal Body 9. Dimension: NA 10. Model/Catalogue No./Name :STARNUKE-MX100 - Diagnostic Mobile X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,XRAYINDIA 100M - Diagnostic Mobile X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,RadX-100M - Diagnostic Mobile X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,STARNUKE-MX100 Mobile Digital Radiography System - Diagnostic Mobile Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,XRAYINDIA 100M Mobile Digital Radiography System - Diagnostic Mobile Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW ,RadX-100M Mobile Digital Radiography System - Diagnostic Mobile Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW

6	1. Generic Name :X-Ray Machine Radiography (Fixed) LF 2. Brand Name :STARNUKE 3. Notified Category : X-Ray Machine 4. Class of Medical Device :Class C 5. Shelf life :15 Years 6. Sterile/Non-Sterile:Non-Sterilized 7. Intended Use :It is used to diagnose or treat patients by recording images of the internal structure of the body to assess the presence or absence of disease, foreign objects, and structural damage or anomaly. 8. Material of Construction: Metal Body 9. Dimension: NA 10. Model/Catalogue No./Name :STARNUKE-FX100 - Diagnostic Fixed X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Peak Output Voltage 100kVp output power 8kW with Table , STARNUKE-FX300 - Diagnostic X-ray machine Permanently Installed type Six Pulse Line Frequency Generator For rated line voltage 230 ± 10 V frequency 50 Hz Three phase Current 300 mA Rated Peak Output Voltage 125 kVp Output power 24 kW with Table , XRAYINDIA 100F - Diagnostic Fixed X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table , RadX-100F - Diagnostic Fixed X-ray machine Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table , STARNUKE-FX100 Digital Radiography System - Diagnostic Fixed Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table ,STARNUKE-FX300 Digital Radiography System - Diagnostic Fixed Digital Radiography System Permanently Installed type Six Pulse Line Frequency Generator For rated line voltage 230 ± 10 V frequency 50 Hz Three phase Current 300 mA Rated Peak Output Voltage 125 kVp Output power 24 kW with Table ,XRAYINDIA 100F Digital Radiography System - Diagnostic Fixed Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table ,RadX-100F Digital Radiography System - Diagnostic Fixed Digital Radiography System Two Pulse type Line frequency generator for rated line voltage 230V frequency 50Hz Single phase current 100mA Rated Peak Output Voltage 100kVp output power 8kW with Table
---	---

Note: Validity of the Market Satanding will be 1 year from the date of issuance or till validity of licence,whichever is earlier.

This is an online-generated permission therefore, a digital signature is not required.



National Accreditation Board for
Testing and Calibration Laboratories

CERTIFICATE OF ACCREDITATION

**STAR NUKE CONSULTING ENGINEERING SERVICES PVT.
LTD.**

has been assessed and accredited in accordance with the standard

ISO/IEC 17025:2017

**"General Requirements for the Competence of Testing &
Calibration Laboratories"**

for its facilities at

PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR,
RAJASTHAN, INDIA

in the field of

TESTING

Certificate Number: TC-11216

Issue Date: 16/12/2024

Valid Until: 15/12/2028

This certificate remains valid for the Scope of Accreditation as specified in the annexure subject to continued
satisfactory compliance to the above standard & the relevant requirements of NABL.

(To see the scope of accreditation of this laboratory, you may also visit NABL website www.nabl-india.org)

Name of Legal Entity: STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED

Signed for and on behalf of NABL



Pankaj Johri
Director

N. Venkateswaran
Chief Executive Officer



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard ISO/IEC 17025:2017

Certificate Number TC-11216

Page No 1 of 16

Validity 16/12/2024 to 15/12/2028

Last Amended on 28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
Permanent Testing				
1	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Alignment of Table to Gantry	AERB/RF-MED/SC-03
2	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Gantry Tilt	AERB/RF-MED/SC-03
3	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	High Contrast Resolution	AERB/RF-MED/SC-03
4	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Linearity of Radiation Output (mA/ mAs Linearity) (CoL)	AERB/RF-MED/SC-03
5	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Low Contrast Resolution	AERB/RF-MED/SC-03
6	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Operating Potential	AERB/RF-MED/SC-03
7	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Radiation Dose Test [Weighted Computed Tomography Dose Index (CTDIW) for Head and Body Phantom]	AERB/RF-MED/SC-03
8	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Radiation Leakage Level from X-Ray Tube Housing	AERB/RF-MED/SC-03
9	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Radiation Protection Survey	AERB/RF-MED/SC-03
10	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Reproducibility of Output (CoV)	AERB/RF-MED/SC-03
11	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Slice Thickness	AERB/RF-MED/SC-03
12	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Table Indexing	AERB/RF-MED/SC-03
13	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Timer	AERB/RF-MED/SC-03
14	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Total Filtration	AERB/RF-MED/SC-03

This is annexure to 'Certificate of Accreditation' and does not require any signature.



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard ISO/IEC 17025:2017

Certificate Number TC-11216

Page No 2 of 16

Validity 16/12/2024 to 15/12/2028

Last Amended on 28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
15	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Consistency of Radiation Output (CoV)	AERB/RF-MED/SC-03
16	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	High Contrast Resolution	AERB/RF-MED/SC-03
17	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Irradiation Time	AERB/RF-MED/SC-03
18	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Linearity of mA/mAs Loading Stations (CoL)	AERB/RF-MED/SC-03
19	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Low Contrast Resolution	AERB/RF-MED/SC-03
20	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Operating Potential	AERB/RF-MED/SC-03
21	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Radiation Dose Test (CTDI)	AERB/RF-MED/SC-03
22	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Radiation Leakage Level from X-ray Tube Housing at 1m from the focus	AERB/RF-MED/SC-03
23	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Radiation Protection Survey	AERB/RF-MED/SC-03
24	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Total Filtration	AERB/RF-MED/SC-03
25	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Exposure Rate at Tabletop	AERB/RF-MED/SC-03
26	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	High contrast sensitivity	AERB/RF-MED/SC-03
27	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Irradiation Timer	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

3 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
28	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Linearity of mA/mAs loading Stations (CoL)	AERB/RF-MED/SC-03
29	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Low contrast resolution	AERB/RF-MED/SC-03
30	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Operating Potential (kV)	AERB/RF-MED/SC-03
31	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Radiation Leakage level from X-Ray tube housing	AERB/RF-MED/SC-03
32	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Radiation Protection Survey of the installation	AERB/RF-MED/SC-03
33	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Reproducibility of Radiation Output (CoV)	AERB/RF-MED/SC-03
34	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Total Filtration	AERB/RF-MED/SC-03
35	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Exposure Rate at Tabletop	AERB/RF-MED/SC- 03
36	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	High Contrast Resolution	AERB/RF-MED/SC- 03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO
25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER,
JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

4 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
37	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Irradiation Timer	AERB/RF-MED/SC- 03
38	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Linearity of mA/mAs Loading station (CoL)	AERB/RF-MED/SC- 03
39	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Low Contrast Resolution	AERB/RF-MED/SC- 03
40	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Operating Potential (kV)	AERB/RF-MED/SC- 03
41	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Radiation leakage level at 1m from tube housing and Collimator	AERB/RF-MED/SC- 03
42	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Radiation Protection Survey of the installation	AERB/RF-MED/SC- 03
43	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Reproducibility of Radiation Output (CoV)	AERB/RF-MED/SC- 03
44	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Total Filtration	AERB/RF-MED/SC- 03
45	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Congruence of radiation and Optical field	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO
25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER,
JAIPUR, RAJASTHAN, INDIA

Accreditation Standard ISO/IEC 17025:2017

Certificate Number TC-11216

Page No 5 of 16

Validity 16/12/2024 to 15/12/2028

Last Amended on 28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
46	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	' Linearity of mA/mAs Loading station (CoL)	AERB/RF-MED/SC- 03
47	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Central Beam Alignment	AERB/RF-MED/SC-03
48	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Effective Focal Spot	AERB/RF-MED/SC-03
49	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Exposure Rate at Tabletop	AERB/RF-MED/SC- 03
50	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	High Contrast resolution	AERB/RF-MED/SC- 03
51	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Irradiation Timer	AERB/RF-MED/SC- 03
52	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Low Contrast Resolution	AERB/RF-MED/SC- 03
53	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Operating Potential (kV)	AERB/RF-MED/SC- 03
54	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Radiation leakage level at 1m from tube housing and Collimator	AERB/RF-MED/SC- 03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO
25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER,
JAIPUR, RAJASTHAN, INDIA

Accreditation Standard ISO/IEC 17025:2017

Certificate Number TC-11216

Page No 6 of 16

Validity 16/12/2024 to 15/12/2028

Last Amended on 28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
55	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Radiation Protection Survey of the installation	AERB/RF-MED/SC- 03
56	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Reproducibility of Radiation Output (CoV)	AERB/RF-MED/SC- 03
57	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Total Filtration	AERB/RF-MED/SC- 03
58	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Linearity of mA/mAs (CoL)	AERB/RF-MED/SC-03
59	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Operating Potential	AERB/RF-MED/SC-03
60	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Performance of imaging phantom	AERB/RF-MED/SC-03
61	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Radiation Leakage level from X-Ray tube housing	AERB/RF-MED/SC-03
62	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Radiation Protection Survey of the installation	AERB/RF-MED/SC-03
63	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Reproducibility of output (CoV)	AERB/RF-MED/SC-03
64	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Timer	AERB/RF-MED/SC-03
65	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Total Filtration	AERB/RF-MED/SC-03
66	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Consistency of Radiation Output (CoV)	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard ISO/IEC 17025:2017

Certificate Number TC-11216

Page No 7 of 16

Validity 16/12/2024 to 15/12/2028

Last Amended on 28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
67	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Irradiation Time	AERB/RF-MED/SC-03
68	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Linearity of mA/mAs Loading Stations (CoL)	AERB/RF-MED/SC-03
69	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Operating Potential	AERB/RF-MED/SC-03
70	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Radiation Leakage Level from X-ray Tube Housing at 1m from the focus	AERB/RF-MED/SC-03
71	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Radiation Protection Survey	AERB/RF-MED/SC-03
72	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Total Filtration	AERB/RF-MED/SC-03
73	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Consistency of radiation output (CoV)	AERB/RF-MED/SC-03
74	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Linearity of mA/mAs loading Stations (CoL)	AERB/RF-MED/SC-03
75	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Central Beam Alignment	AERB/RF-MED/SC-03
76	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Congruence of radiation and Optical field	AERB/RF-MED/SC-03
77	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Effective focal spot	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO
25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER,
JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

8 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
78	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Total Filtration	AERB/RF-MED/SC-03
79	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Irradiation Time	AERB/RF-MED/SC-03
80	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Operating Potential	AERB/RF-MED/SC-03
81	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Radiation leakage level at 1m from tube housing and Collimator	AERB/RF-MED/SC-03
82	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Radiation Protection Survey of the installation	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

9 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
Site Testing				
1	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Alignment of Table to Gantry	AERB/RF-MED/SC-03
2	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Gantry Tilt	AERB/RF-MED/SC-03
3	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	High Contrast Resolution	AERB/RF-MED/SC-03
4	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Linearity of Radiation Output (mA/ mAs Linearity) (CoL)	AERB/RF-MED/SC-03
5	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Low Contrast Resolution	AERB/RF-MED/SC-03
6	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Operating Potential	AERB/RF-MED/SC-03
7	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Radiation Dose Test [Weighted Computed Tomography Dose Index (CTDIW) for Head and Body Phantom]	AERB/RF-MED/SC-03
8	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Radiation Leakage Level from X-Ray Tube Housing	AERB/RF-MED/SC-03
9	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Radiation Protection Survey	AERB/RF-MED/SC-03
10	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Reproducibility of Output (CoV)	AERB/RF-MED/SC-03
11	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Slice Thickness	AERB/RF-MED/SC-03
12	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Table Indexing	AERB/RF-MED/SC-03
13	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Timer	AERB/RF-MED/SC-03
14	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	CT Equipment	Total Filtration	AERB/RF-MED/SC-03

This is annexure to 'Certificate of Accreditation' and does not require any signature.



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO
25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER,
JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

10 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
15	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Consistency of Radiation Output (CoV)	AERB/RF-MED/SC-03
16	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	High Contrast Resolution	AERB/RF-MED/SC-03
17	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Irradiation Time	AERB/RF-MED/SC-03
18	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Linearity of mA/mAs Loading Stations (CoL)	AERB/RF-MED/SC-03
19	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Low Contrast Resolution	AERB/RF-MED/SC-03
20	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Operating Potential	AERB/RF-MED/SC-03
21	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Radiation Dose Test (CTDI)	AERB/RF-MED/SC-03
22	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Radiation Leakage Level from X-ray Tube Housing at 1m from the focus	AERB/RF-MED/SC-03
23	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Radiation Protection Survey	AERB/RF-MED/SC-03
24	DIAGNOSTIC RADIOLOGY QA TESTING- COMPUTED TOMOGRAPHY (CT)	DENTAL CONE BEAM CT	Total Filtration	AERB/RF-MED/SC-03
25	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Exposure Rate at Tabletop	AERB/RF-MED/SC-03
26	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	High contrast sensitivity	AERB/RF-MED/SC-03
27	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Irradiation Timer	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

11 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
28	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Linearity of mA/mAs loading Stations (CoL)	AERB/RF-MED/SC-03
29	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Low contrast resolution	AERB/RF-MED/SC-03
30	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Operating Potential (kV)	AERB/RF-MED/SC-03
31	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Radiation Leakage level from X-Ray tube housing	AERB/RF-MED/SC-03
32	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Radiation Protection Survey of the installation	AERB/RF-MED/SC-03
33	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Reproducibility of Radiation Output (CoV)	AERB/RF-MED/SC-03
34	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	C Arm	Total Filtration	AERB/RF-MED/SC-03
35	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Exposure Rate at Tabletop	AERB/RF-MED/SC- 03
36	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	High Contrast Resolution	AERB/RF-MED/SC- 03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

12 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
37	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Irradiation Timer	AERB/RF-MED/SC- 03
38	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Linearity of mA/mAs Loading station (CoL)	AERB/RF-MED/SC- 03
39	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Low Contrast Resolution	AERB/RF-MED/SC- 03
40	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Operating Potential (kV)	AERB/RF-MED/SC- 03
41	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Radiation leakage level at 1m from tube housing and Collimator	AERB/RF-MED/SC- 03
42	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Radiation Protection Survey of the installation	AERB/RF-MED/SC- 03
43	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Reproducibility of Radiation Output (CoV)	AERB/RF-MED/SC- 03
44	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Cath Lab	Total Filtration	AERB/RF-MED/SC- 03
45	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Congruence of radiation and Optical field	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

13 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
46	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	' Linearity of mA/mAs Loading station (CoL)	AERB/RF-MED/SC- 03
47	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Central Beam Alignment	AERB/RF-MED/SC-03
48	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Effective Focal Spot	AERB/RF-MED/SC-03
49	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Exposure Rate at Tabletop	AERB/RF-MED/SC- 03
50	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	High Contrast resolution	AERB/RF-MED/SC- 03
51	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Irradiation Timer	AERB/RF-MED/SC- 03
52	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Low Contrast Resolution	AERB/RF-MED/SC- 03
53	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Operating Potential (kV)	AERB/RF-MED/SC- 03
54	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Radiation leakage level at 1m from tube housing and Collimator	AERB/RF-MED/SC- 03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO
25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER,
JAIPUR, RAJASTHAN, INDIA

Accreditation Standard ISO/IEC 17025:2017

Certificate Number TC-11216

Page No 14 of 16

Validity 16/12/2024 to 15/12/2028

Last Amended on 28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
55	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Radiation Protection Survey of the installation	AERB/RF-MED/SC- 03
56	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Reproducibility of Radiation Output (CoV)	AERB/RF-MED/SC- 03
57	DIAGNOSTIC RADIOLOGY QA TESTING- INTERVENTIONAL RADIOLOGY & FLUOROSCOPY	Radiography & Fluoroscopy Machine	Total Filtration	AERB/RF-MED/SC- 03
58	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Linearity of mA/mAs (CoL)	AERB/RF-MED/SC-03
59	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Operating Potential	AERB/RF-MED/SC-03
60	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Performance of imaging phantom	AERB/RF-MED/SC-03
61	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Radiation Leakage level from X-Ray tube housing	AERB/RF-MED/SC-03
62	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Radiation Protection Survey of the installation	AERB/RF-MED/SC-03
63	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Reproducibility of output (CoV)	AERB/RF-MED/SC-03
64	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Timer	AERB/RF-MED/SC-03
65	DIAGNOSTIC RADIOLOGY QA TESTING- MAMMOGRAPHY	Mammography	Total Filtration	AERB/RF-MED/SC-03
66	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Consistency of Radiation Output (CoV)	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard ISO/IEC 17025:2017

Certificate Number TC-11216

Page No 15 of 16

Validity 16/12/2024 to 15/12/2028

Last Amended on 28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
67	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Irradiation Time	AERB/RF-MED/SC-03
68	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Linearity of mA/mAs Loading Stations (CoL)	AERB/RF-MED/SC-03
69	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Operating Potential	AERB/RF-MED/SC-03
70	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Radiation Leakage Level from X-ray Tube Housing at 1m from the focus	AERB/RF-MED/SC-03
71	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Radiation Protection Survey	AERB/RF-MED/SC-03
72	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	DENTAL (INTRA ORAL), DENTAL (HAND-HELD), ORTHO PANTOMOGRAPHY (OPG), BONE DENSITOMETER (BMD)	Total Filtration	AERB/RF-MED/SC-03
73	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Consistency of radiation output (CoV)	AERB/RF-MED/SC-03
74	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Linearity of mA/mAs loading Stations (CoL)	AERB/RF-MED/SC-03
75	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Central Beam Alignment	AERB/RF-MED/SC-03
76	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Congruence of radiation and Optical field	AERB/RF-MED/SC-03
77	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Effective focal spot	AERB/RF-MED/SC-03



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

STAR NUKE CONSULTING ENGINEERING SERVICES PVT. LTD., PLOT NO 25, NAVKAR NAGAR, KALYANPURA, NEW SANGANER ROAD, SANGANER, JAIPUR, RAJASTHAN, INDIA

Accreditation Standard

ISO/IEC 17025:2017

Certificate Number

TC-11216

Page No

16 of 16

Validity

16/12/2024 to 15/12/2028

Last Amended on

28/01/2025

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
78	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Total Filtration	AERB/RF-MED/SC-03
79	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Irradiation Time	AERB/RF-MED/SC-03
80	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Operating Potential	AERB/RF-MED/SC-03
81	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Radiation leakage level at 1m from tube housing and Collimator	AERB/RF-MED/SC-03
82	DIAGNOSTIC RADIOLOGY QA TESTING- RADIOGRAPHY (X-RAY - FIXED PORTABLE, MOBILE)	X- Ray Equipment (Fixed, Portable & Mobile)	Radiation Protection Survey of the installation	AERB/RF-MED/SC-03



Government of India

Form GST REG-06

[See Rule 10(1)]

Registration Certificate

Registration Number : 08AAVCS3158D2ZZ

1.	Legal Name	STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED			
2.	Trade Name, if any	STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE LIMITED			
3.	Additional trade names, if any				
4.	Constitution of Business	Private Limited Company			
5.	Address of Principal Place of Business	Building No./Flat No.: Plot No. 25 Name Of Premises/Building: Navkar Nagar Road/Street: New Sanganer Road City/Town/Village: Kalyanpura, Sanganer District: Jaipur State: Rajasthan PIN Code: 302020			
6.	Date of Liability	01/08/2017			
7.	Date of Validity	From	11/09/2017	To	Not Applicable
8.	Type of Registration	Regular			
9.	Particulars of Approving	Rajasthan Goods and Services Tax Act, 2017			

Signature

Signature Not Verified

 Digitally signed by DS GOODS
 AND SERVICES TAX
 NETWORK 07
 Date: 2024.08.07 15:00:56 IST

Name	KALPANA BANSAL
Designation	Assistant Commissioner
Jurisdictional Office	Circle-A, Kota - Ward-II
Date of issue of Certificate	07/08/2024

Note: The registration certificate is required to be prominently displayed at all places of Business/Office(s) in the State.

This is a system generated digitally signed Registration Certificate issued based on the approval of application granted on 07/08/2024 by the jurisdictional authority.



Goods and Services Tax Identification Number: 08AAVCS3158D2ZZ

Details of Additional Place of Business(s)

Legal Name STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE

Trade Name, if any STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE

Additional trade names, if any

Total Number of Additional Places of Business(s) in the State 1

- 1 27 Radha Nikunj B, Kharbas Circle Road, Near Escon Temple, Mansarovar, Jaipur, Jaipur, Rajasthan, 302020



Goods and Services Tax Identification Number: 08AAVCS3158D2ZZ

Legal Name STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE

Trade Name, if any STAR NUKE CONSULTING ENGINEERING SERVICES PRIVATE

Additional trade names, if any

Details of Managing / Whole-time Directors and Key Managerial Persons

1		Name	USHA RAO
		Designation/Status	DIRECTOR
		Resident of State	Rajasthan
2		Name	Balram Singh Rajora
		Designation/Status	Director
		Resident of State	Rajasthan





Star Nuke Consulting Engineering Service Private Limited

ISO 9001-2015 Certified company

OUR BANK PARTICULARS FOR BANK & WIRE PAYMENT INCLUDING ELECTRONIC FUNDS TRANSFER (EFT)

- | | |
|------------------------|---|
| • NAME OF THE BANK: | HDFC BANK LIMITED |
| • BANK ADDRESS: | GROUND FLOOR, 69,399, MADHYAM MARG,
MANSAROVAR, JAIPUR, RAJASTHAN - 302020 |
| • BRANCH CODE: | 7041 |
| • BENEFICIARY NAME: | STAR NUKE CONS. ENG. SERVICES PVT. LTD. |
| • BENEFICIARY A/C NO.: | 50200078360103 |
| • ACCOUNT TYPE: | CURRENT |
| • IFSC CODE: | HDFC0007041 |

STAR NUKE CONS. ENG. SERVICES
PVT. LTD.

AUTHORIZED SIGNATORY

Star Nuke Consulting
Engineering Services Pvt. Ltd.
[Signature]
Authorised Signatory

HDFC BANK LIMITED

BRANCH MANAGER

[Signature]
Ruma Bhatnagar
Branch Manager
Emp. Code: R103
Madhyam Marg, Mansarovar-3741



HDFC BANK LTD, GROUND FLOOR, 69,399,
MADHYAM MARG, MANSAROVAR, JAIPUR-302020, RAJASTHAN
RTGS / NEFT IFSC : HDFC0007041

--	--	--	--	--	--	--	--

D D M M Y Y Y Y

Valid for 3 months only

Or Bearer

Pay

या धारक को

Rupees रुपये

अदा करें

₹

A/c. No.

खाता नं.

50200078360103

Brn: 7041 Pdt: (New Account)
CURRENT

For STAR NUKE CONS ENG SERVICES PVT LTD

Payable at par through clearing/transfer in branches of HDFC BANK LTD

Authorised Signatories

Please sign above / कृपया यहाँ हस्ताक्षर करें

0000004 30224006 001290 29