


Lab01 - Session 01
 Δ_{47} repeatability = 31.4 ppm

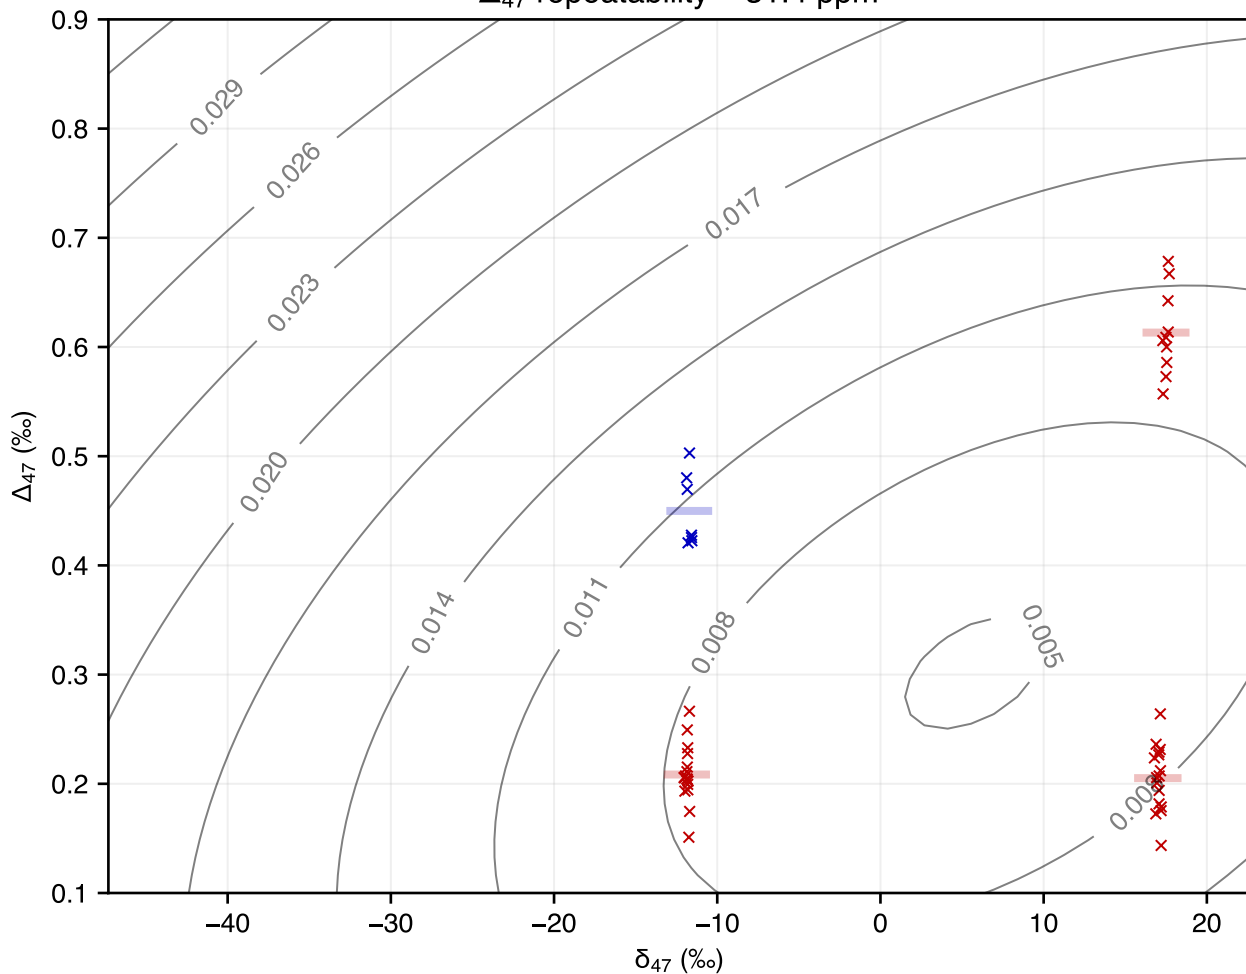

All analyses (cross markers) in Session 01 of Lab 01.
Anchors are plotted in red and unknown in blue.
Average Δ_{47} values for each sample are plotted as thick blue and red lines.
Standardization errors are mapped as grey contours.