


Lab14 - Session 09
 Δ_{47} repeatability = 12.0 ppm

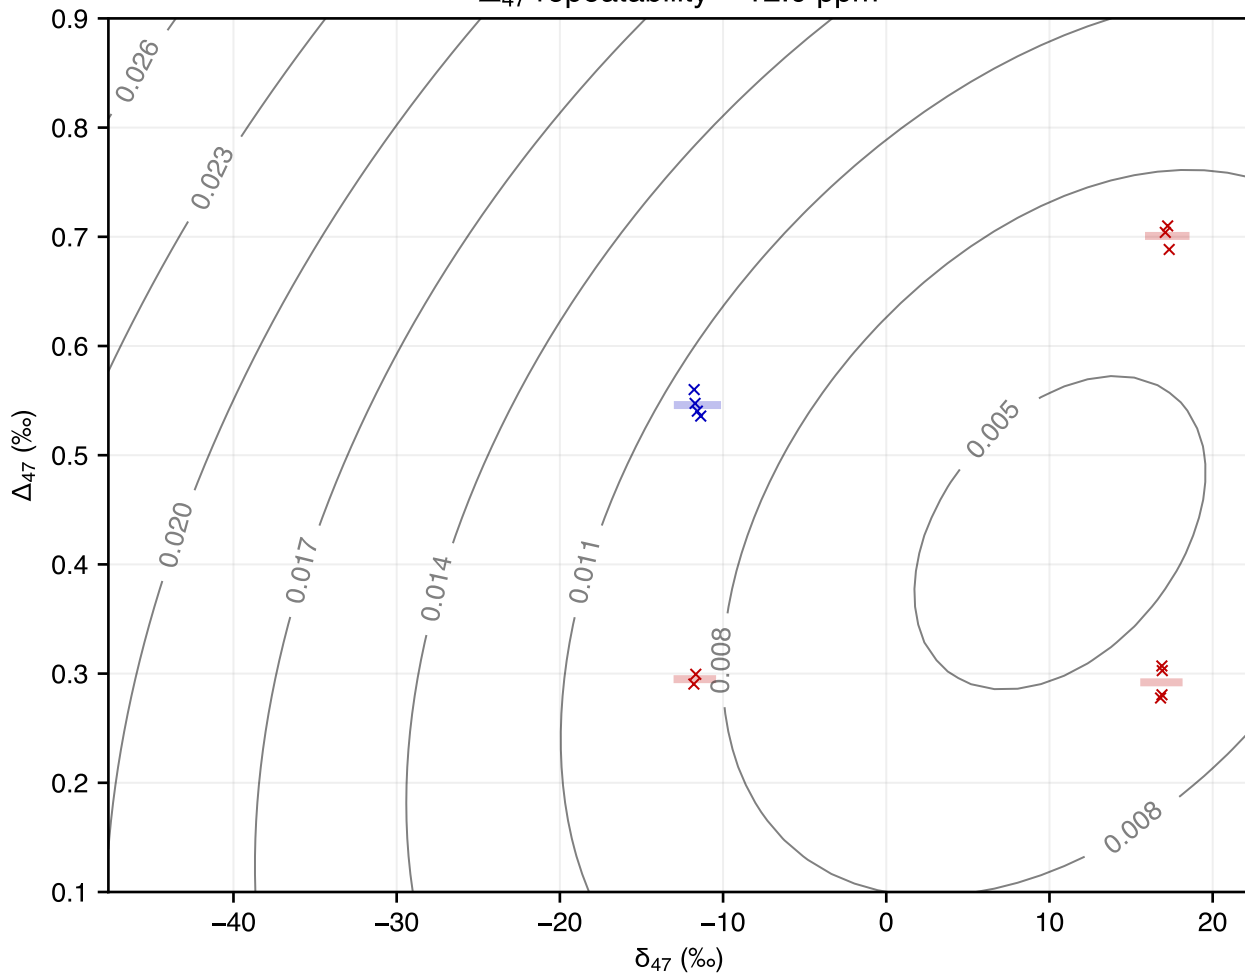

All analyses (cross markers) in Session 09 of Lab 14.
Anchors are plotted in red and unknown in blue.
Average Δ_{47} values for each sample are plotted as thick blue and red lines.
Standardization errors are mapped as grey contours.