


Lab11 - Session 02
 Δ_{47} repeatability = 28.9 ppm

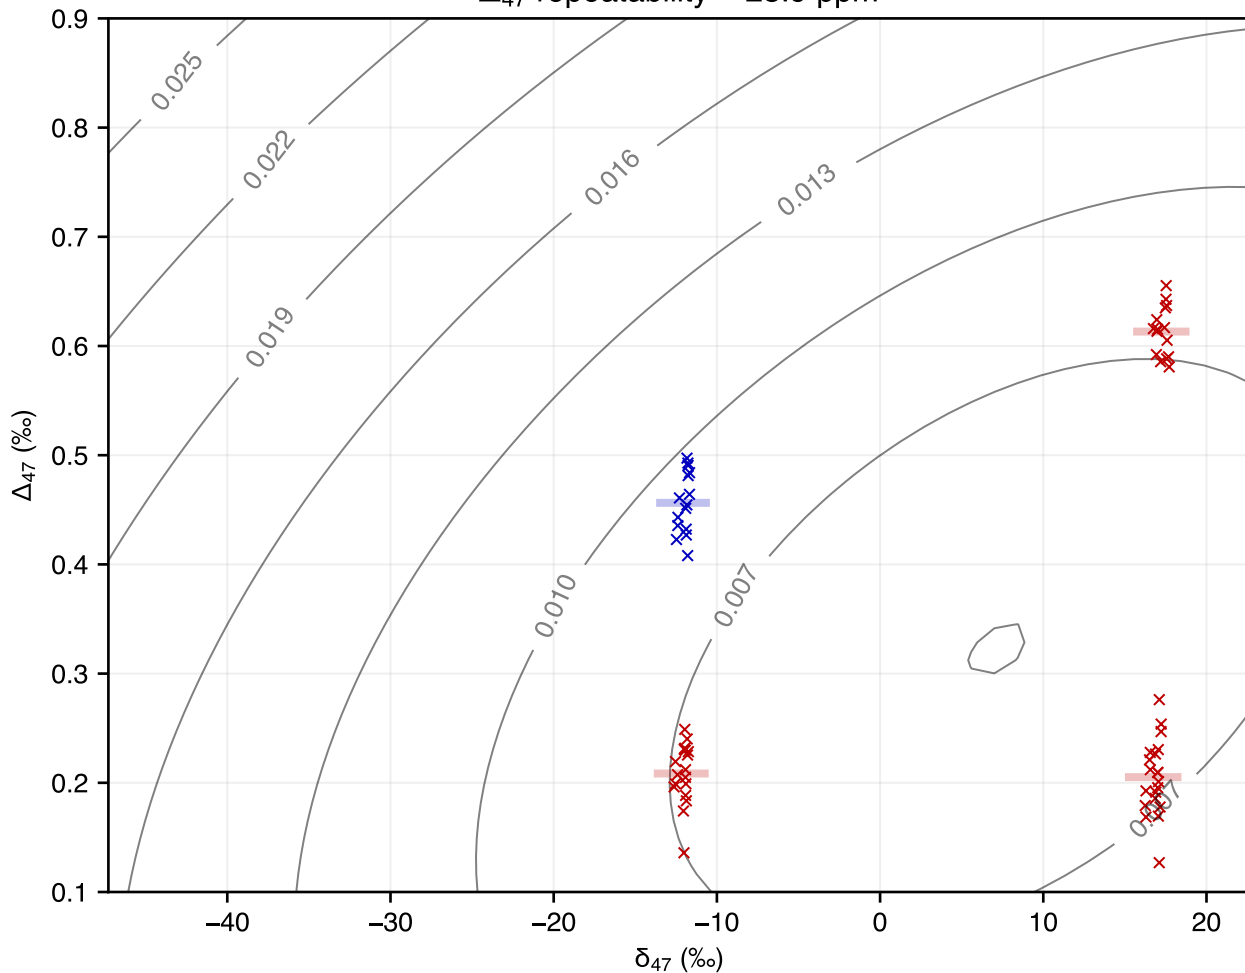

All analyses (cross markers) in Session 02 of Lab 11.
 Anchors are plotted in red and unknown in blue.
 Average Δ_{47} values for each sample are plotted as thick blue and red lines.
 Standardization errors are mapped as gray contours.