


Lab26 - Session 01
 Δ_{47} repeatability = 15.0 ppm

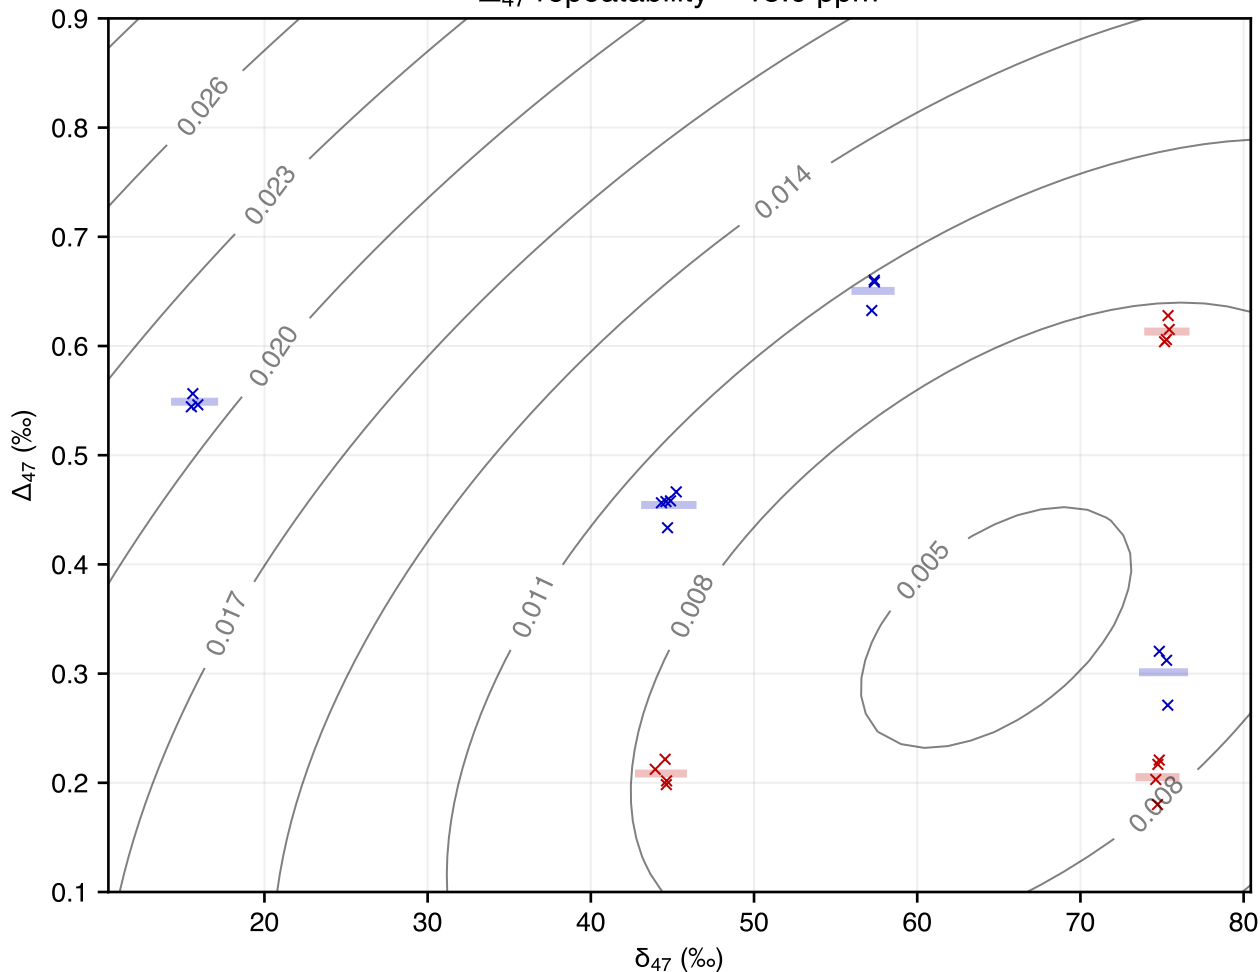

All analyses (cross markers) in Session 01 of Lab 26.
 Anchors are plotted in red and unknown in blue.
 Average Δ_{47} values for each sample are plotted as thick blue and red lines.
 Standardization errors are mapped as grey contours.