


Lab05 - Session 01
 Δ_{47} repeatability = 8.6 ppm

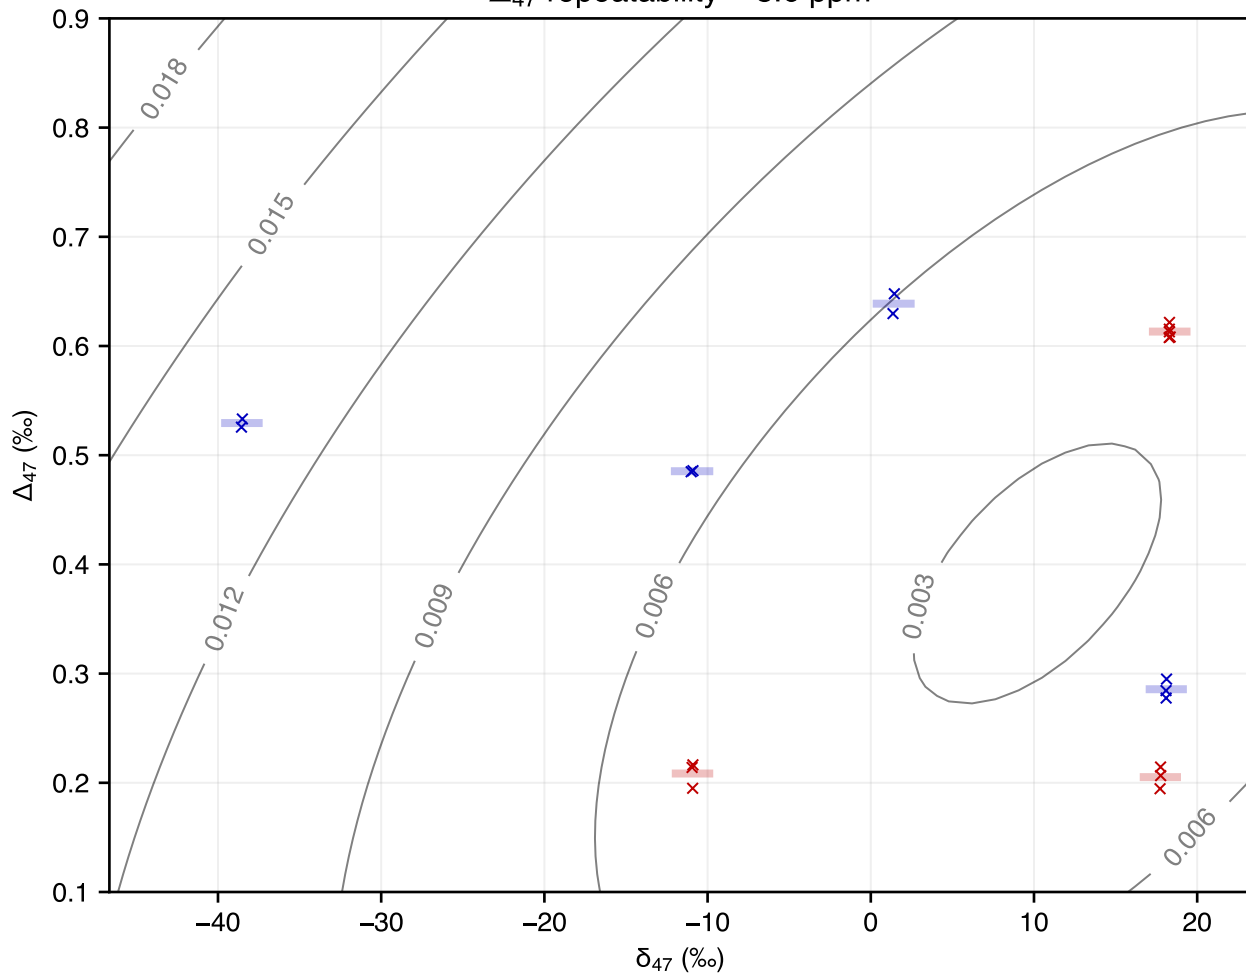

All analyses (cross markers) in Session 01 of Lab 05.
Anchors are plotted in red and unknown in blue.
Average Δ_{47} values for each sample are plotted as thick blue and red lines.
Standardization errors are mapped as gray contours.