


Lab11 - Session 05
 Δ_{47} repeatability = 19.2 ppm

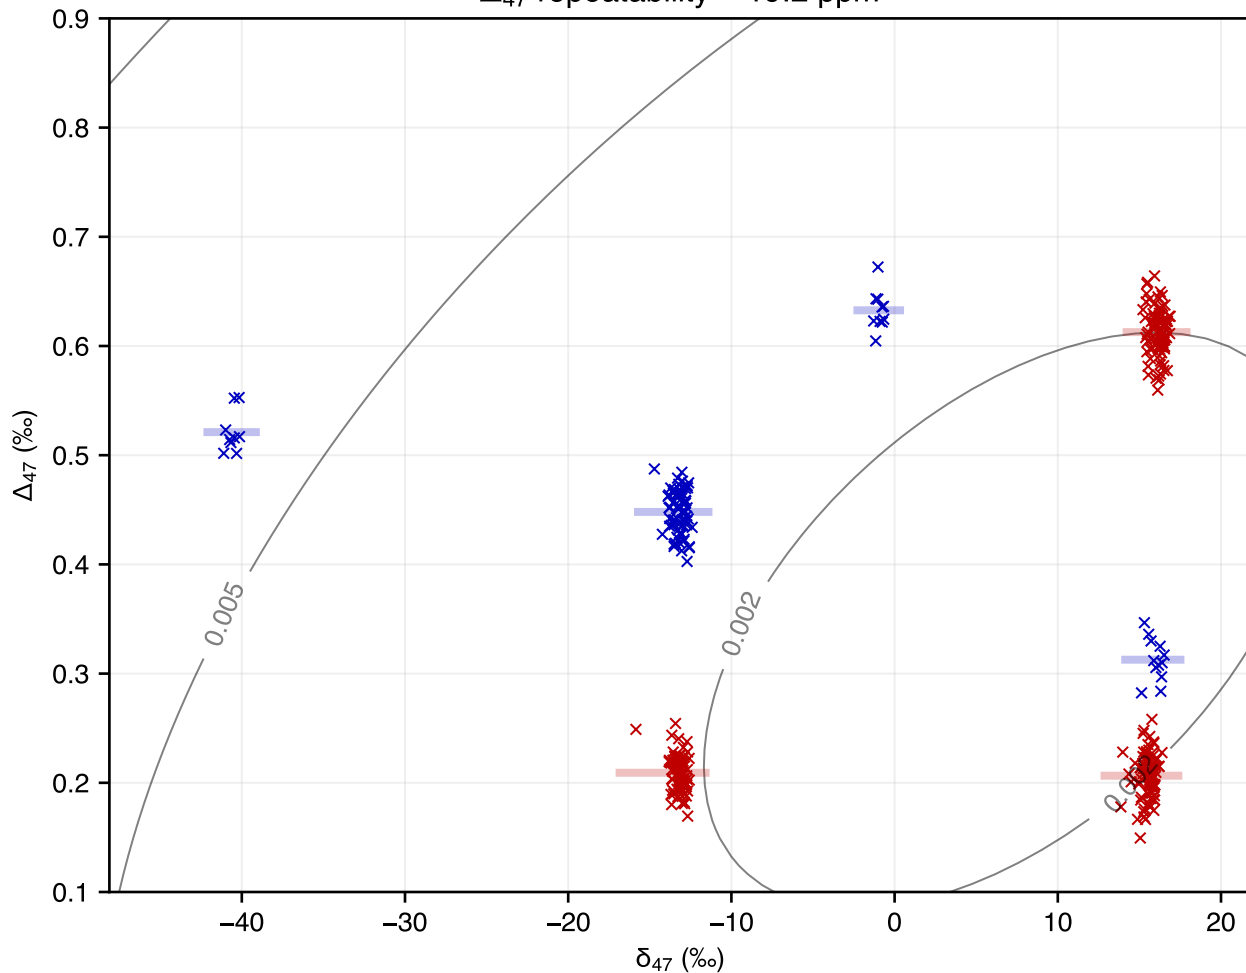

All analyses (cross markers) in Session 05 of Lab 11.
Anchors are plotted in red and unknown in blue.
Average Δ_{47} values for each sample are plotted as thick blue and red lines.
Standardization errors are mapped as gray contours.