


Lab18 - Session 03
 Δ_{47} repeatability = 40.5 ppm

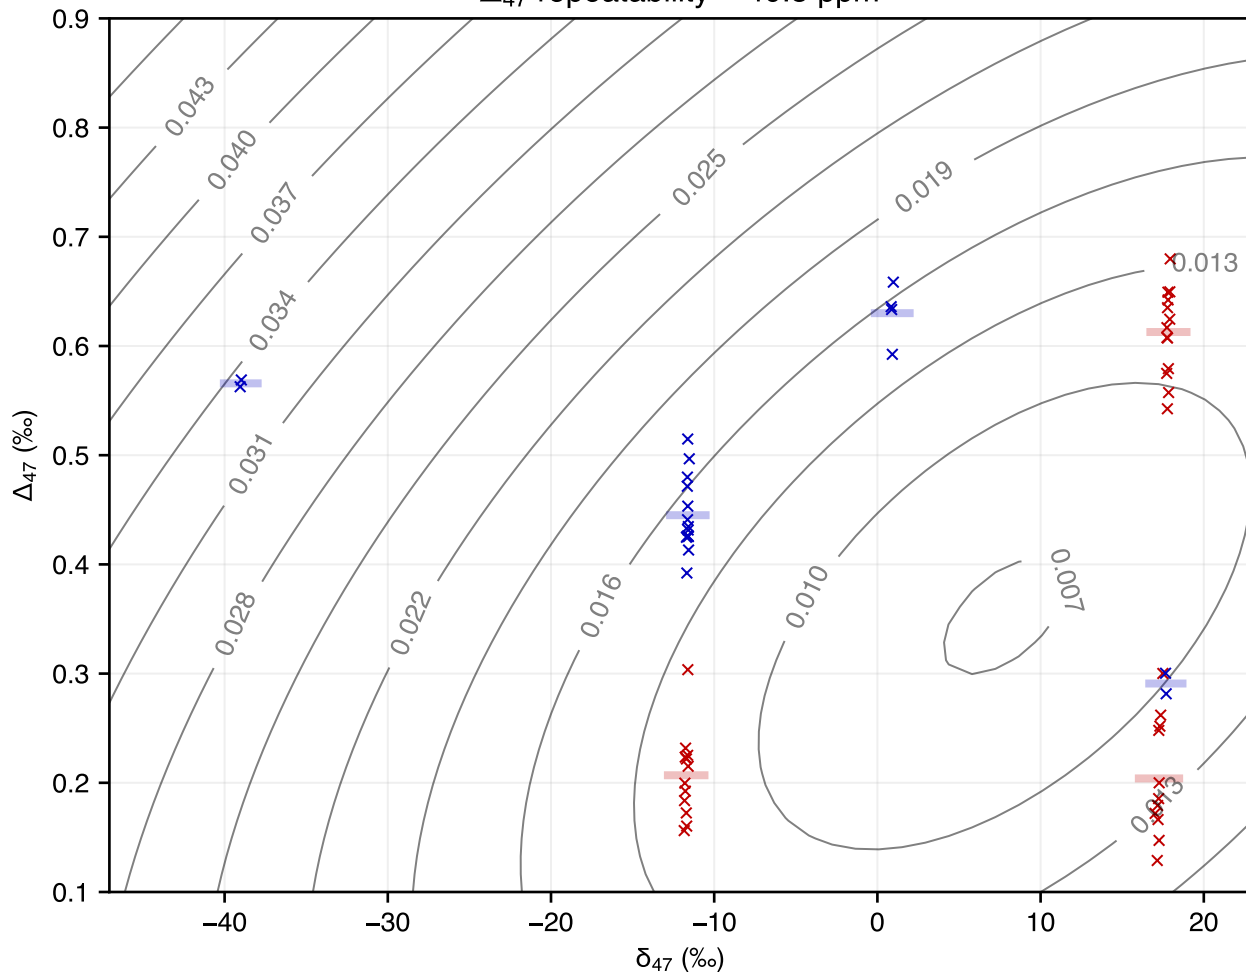

All analyses (cross markers) in Session 03 of Lab 18.
 Anchors are plotted in red and unknown in blue.
 Average Δ_{47} values for each sample are plotted as thick blue and red lines.
 Standardization errors are mapped as grey contours.