


Lab19 - Session 02
 Δ_{47} repeatability = 22.5 ppm

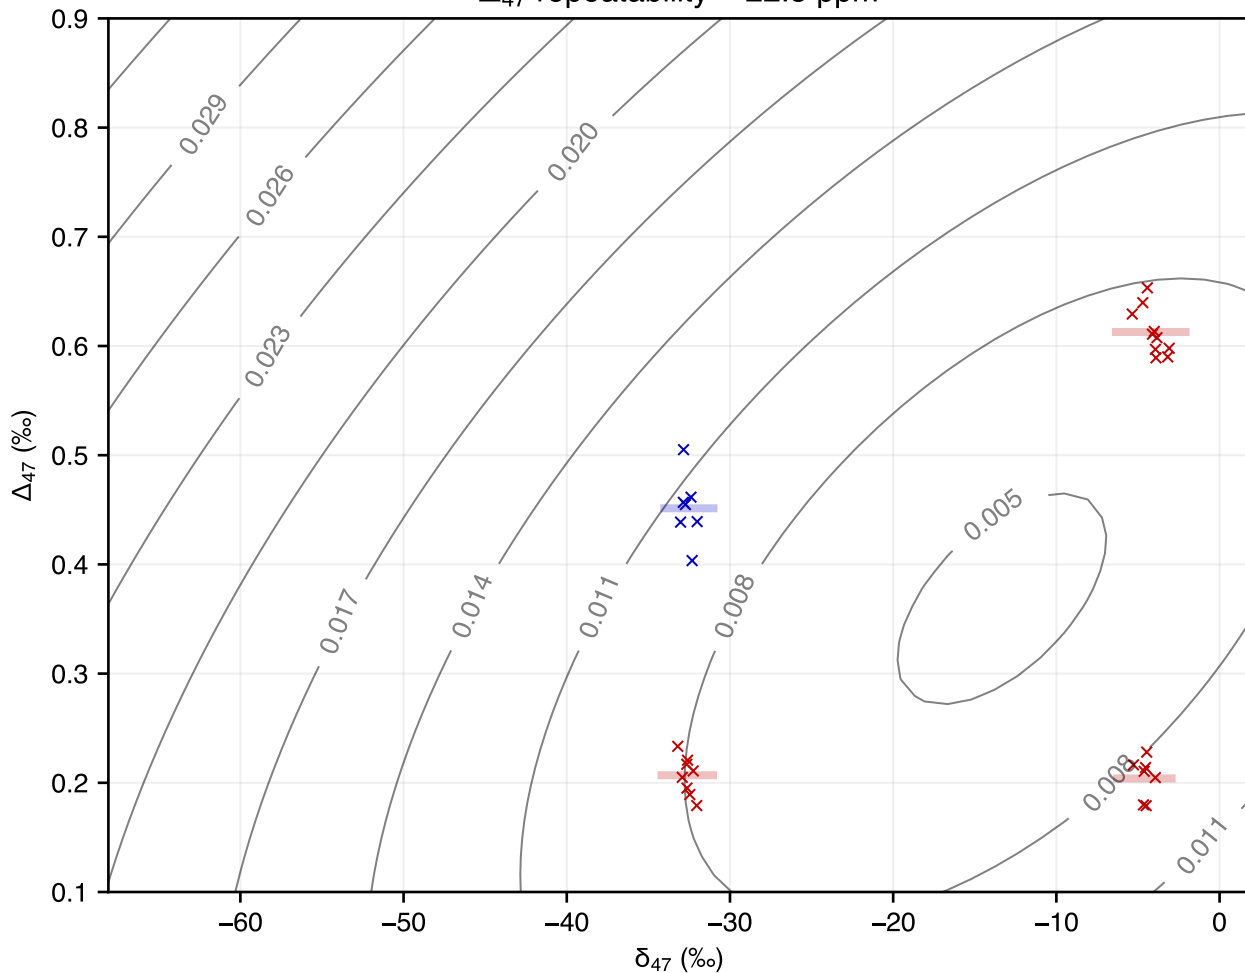

All analyses (cross markers) in Session 02 of Lab 19.
Anchors are plotted in red and unknown in blue.
Average Δ_{47} values for each sample are plotted as thick blue and red lines.
Standardization errors are mapped as grey contours.