


Lab09 - Session 03
 Δ_{47} repeatability = 22.4 ppm

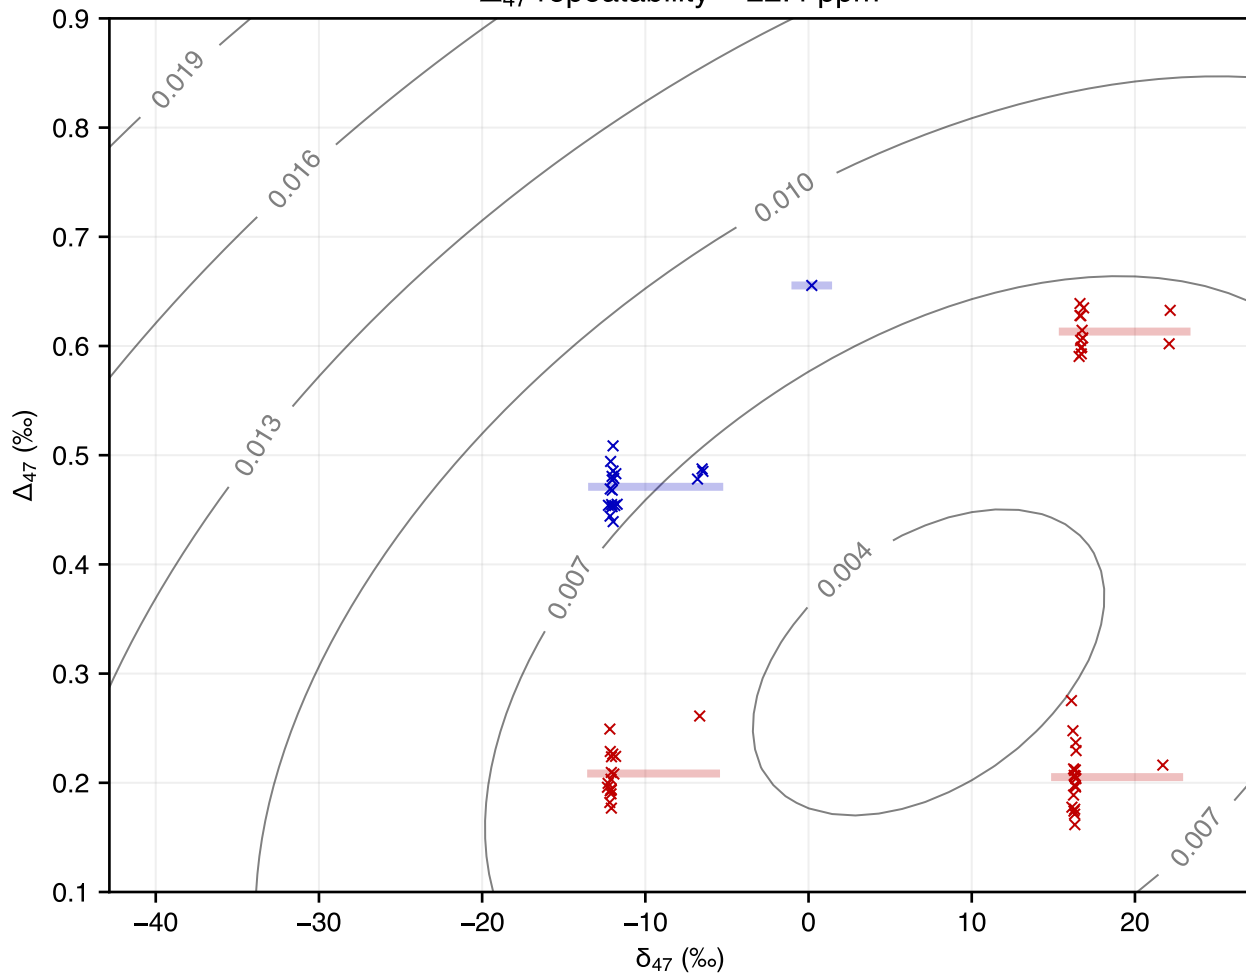

All analyses (cross markers) in Session 03 of Lab 09.
Anchors are plotted in red and unknown in blue.
Average Δ_{47} values for each sample are plotted as thick blue and red lines.
Standardization errors are mapped as grey contours.