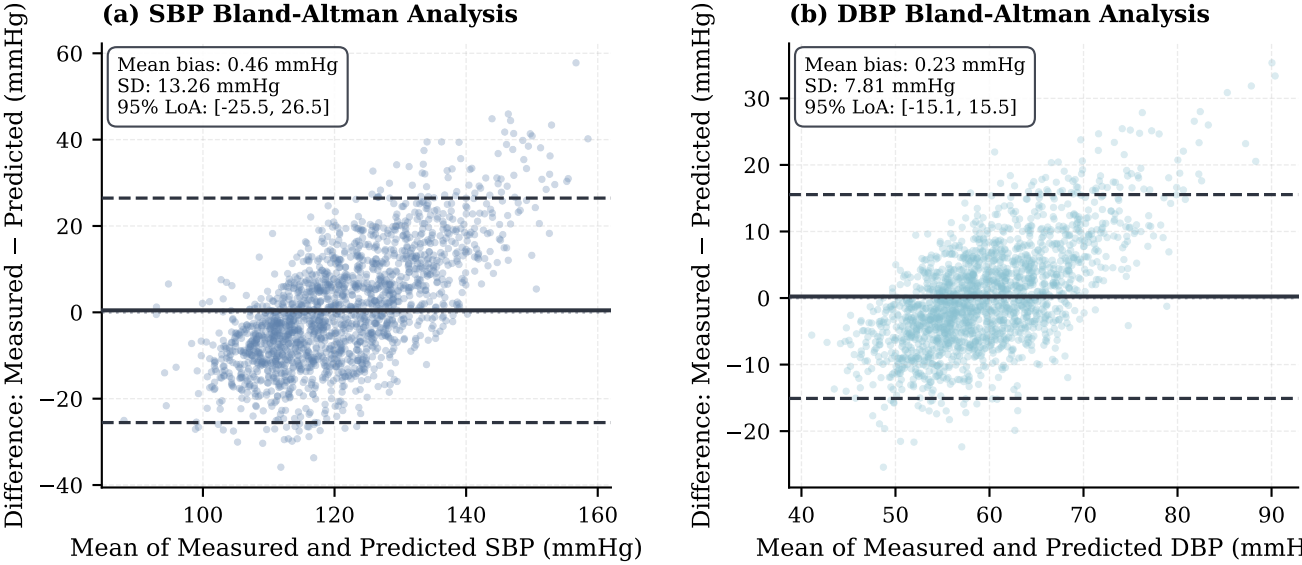

(a) SBP Bland-Altman Analysis
Mean bias: 0.46 mmHg
SD: 13.26 mmHg
95% LoA: [-25.5, 26.5]
Difference: Measured − Predicted (mmHg)
Mean of Measured and Predicted SBP (mmHg)
60
40
20
0
−20
−40
100
120
140
160
(b) DBP Bland-Altman Analysis
Mean bias: 0.23 mmHg
SD: 7.81 mmHg
95% LoA: [-15.1, 15.5]
Difference: Measured − Predicted (mmHg)
Mean of Measured and Predicted DBP (mmH
30
20
10
0
−10
−20
40
50
60
70
80
90