


HPLC-DAD Chromatograms

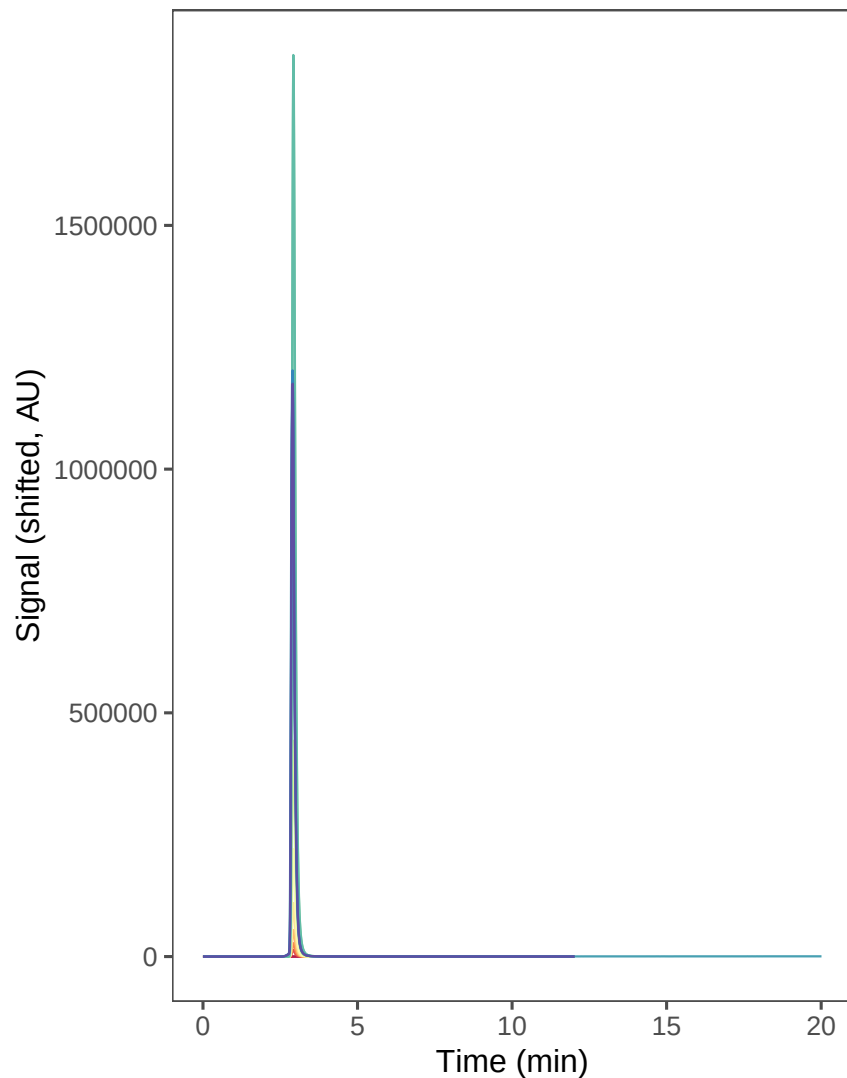

Injection

2026.01.14_BLK_mecn_01	2026.01.14_STD_0.125_mM_02
2026.01.14_BLK_mecn_02	2026.01.14_STD_0.25_mM_01
2026.01.14_STD_0.00878125_mM_01	2026.01.14_STD_0.25_mM_02
2026.01.14_STD_0.00878125_mM_02	2026.01.14_STD_0.5_mM_01
2026.01.14_STD_0.015625_mM_01	2026.01.14_STD_0.5_mM_02
2026.01.14_STD_0.015625_mM_02	2026.01.14_STD_1_mM_01
2026.01.14_STD_0.03125_mM_01	2026.01.14_STD_1_mM_02
2026.01.14_STD_0.03125_mM_02	2026.01.19_SMP_EXT1_01
2026.01.14_STD_0.0625_mM_0	2026.01.19_SMP_EXT1_02
2026.01.14_STD_0.0625_mM_01	2026.01.19_SMP_EXT2_01
2026.01.14_STD_0.125_mM_01	2026.01.19_SMP_EXT2_02