


The Dismutators

Daniel Moreira

“How have living systems, which are based on a common set of biochemical structures and processes and subject to a common set of physical-chemical laws, been able to adapt to the enormously wide spectrum of environmental conditions found in the biosphere?” Peter Hochachka and George Somero – Biochemical Adaptation (2002)



Daniel Moreira

<http://www.mdcscience.com>

More text here.

Contents

Contents	iii
Preface to this Book Series	v
I — Fundamental Concepts	1
1 Analytical Chemistry	3
2 Terminology	5
3 Spectrophotometry Fundamentals	7
3.1 Cuvette <i>versus</i> microplates	7
II — Methodological Approaches	9
4 Assays for Determining Enzyme Activity	11
4.1 Overview of assay types	11
4.2 Specific methodologies	11
5 Sample Preparation	13
5.1 Collection	13
5.2 Preparation	13
5.3 Handling and Storage	13
III — The Dismutators	15
6 Background	17
7 Catalase	19
7.1 Introduction	20
7.2 Quick Reference Protocol	21
7.3 Material	22
7.4 Solutions	23

7.5	Checking H_2O_2 Concentration	24
7.6	Sample Preparation	26
7.7	Assay	26
7.8	Expected Results	29
7.9	Calculations	31
7.10	3-Amino-1,2,4-Triazole	34
7.11	Additional Comments	35
7.12	References	40
8	Superoxide Dismutase	41
	Bibliography	43

Preface to this Book Series

This is a book series of protocol book of methods to measure the activity of antioxidant enzymes, oxidative stress markers, and other related biochemical variables.

More than a decade of experience

The idea is that each volume is self-contained. To do so, some basic concepts are repeated in each volume so that the readers does not need to refer to another volume while reading / using in the lab bench a protocol.

So far, the plan is to have the following volumes:

Volume 1 - The Dismutators

Part I

Fundamental Concepts

CHAPTER

1

Analytical Chemistry

CHAPTER 2

Terminology

Spectrophotometry Fundamentals

3.1 Cuvette *versus* microplates

Part II

Methodological Approaches

Assays for Determining Enzyme Activity

- 4.1 Overview of assay types
- 4.2 Specific methodologies

CHAPTER 5

Sample Preparation

5.1 Collection

5.2 Preparation

5.3 Handling and Storage

Part III

The Dismutators

Background

Here write some brief background information on antioxidant systems, catalase and SOD.

Catalase




Some text for this block.


7.1	Introduction	20
7.2	Quick Reference Protocol	21
7.3	Material	22
7.4	Solutions	23
7.5	Checking H_2O_2 Concentration	24
7.6	Sample Preparation	26
7.7	Assay	26
7.8	Expected Results	29
7.9	Calculations	31
7.10	3-Amino-1,2,4-Triazole	34
7.11	Additional Comments	35
7.12	References	40

7.1 Introduction

Catalase is an antioxidant enzyme present in most aerobic organisms. Its function is to catalyze the decomposition of hydrogen peroxide (H_2O_2) into oxygen (O_2). In animals, catalase is a protein composed of four subunits, each containing an Fe(III)-heme group at its active site. Additionally, a molecule of NADPH is tightly bound to each subunit of mammalian catalase.



The reaction catalyzed by catalase is a dismutation (a type of redox reaction in which the same molecular species is simultaneously oxidized and reduced, forming two different products, one with a higher oxidation state and one with a lower). In the case of catalase, this process occurs in two stages, involving the formation of an intermediate known as compound I.



Measuring catalase activity is crucial in research investigating antioxidant systems and cellular responses to oxidative stress. This is illustrated by observations that inhibition of catalase activity or expression induces oxidative stress (Bagnyukova et al. 2005) or increases sensitivity to other stressors (Ho et al. 2004). Additionally, cells particularly resistant to oxidative stressors show overexpression of catalase (Spitz et al. 1992).

There are various methods to determine catalase activity, for example, by measuring the production of O_2 with an O_2 sensor, measuring the consumption of H_2O_2 with a fluorescent probe molecule, or directly measuring the consumption of H_2O_2 by spectrophotometry. The method for determining catalase activity described in this protocol is one of the most popular and is based on the decomposition of hydrogen peroxide by catalase and the consequent decrease in absorbance at 240 nm (Aebi 1984). The procedure involves adding the sample to a buffered reaction medium containing hydrogen peroxide and measuring the decrease in absorbance over time using a spectrophotometer. Enzyme activity is then calculated based on the rate of decrease in absorbance, which is directly proportional to the amount of hydrogen peroxide decomposed. In this protocol, in addition to serving as the substrate for the enzyme, H_2O_2 acts as the indicator molecule (i.e., the molecule that generates the analytical signal recorded in the assay).

7.2 Quick Reference Protocol

This section provides a quick reference with stock and final concentrations of the reagents (Table 7.1), volumes to be pipetted (Table 7.2), and equipment settings for the readings. The complete protocol is detailed in the next sections.

Table 7.1: Stock and final concentrations of reagents used in the protocol.

Reagent	Stock	Final
Phosphate Buffer + EDTA (pH 7.2)		
Potassium Phosphate	500 mM	50 mM
EDTA	5 mM	0.5 mM
Hydrogen Peroxide	200 mM	10 mM

Table 7.2: Volumes to be added for different readings of the protocol.

Assay	KPi + EDTA (7.2)	Water	Sample	H ₂ O ₂
Zero	80	720	0	0
Assay Blank	80	680	0	40
Sample Assay	80	680 - X*	X*	40
Sample Blank	80	720 - X*	X*	0

* X is the volume of sample, which varies from sample to sample.

Equipment Setup

- **Final Volume:** 800 μ L
- **Wavelength:** 240 nm (quartz cuvette)
- **Reading Mode:** Kinetic
 - **Total Reading Time:** 1 min
 - **Suggested Reading Interval:** 0.1 min
- Use a sample volume that results in $\Delta\text{Abs}_{240}/\text{min}$ between -0.025 and -0.035

7.3 Material

Reagents

- Hydrogen Peroxide (H_2O_2) (200 mM) (Cod. 1857, Dinâmica, Indaiatuba, Brazil)
- Phosphate Buffer (KPi) (500 mM pH 7.2) + EDTA (5 mM):
 - Potassium phosphate monobasic (P0662, Sigma-Aldrich, St. Louis, MO)
 - Potassium phosphate dibasic (P3786, Sigma-Aldrich)
 - Ethylenediaminetetraacetic acid (EDS, Sigma-Aldrich)

Note

The manufacturers and codes listed above are those used to produce the examples shown in this protocol, but similar reagents from other manufacturers can be substituted. Always check the purity and molecular weight of the reagent.

Solvents

- Deionized water

Materials

- Quartz cuvette
- Micropipettes
- Parafilm
- Tips for micropipettes
- Container with ice (to keep solutions and samples on ice throughout the protocol)
- Tubes and glassware for the preparation and storage of solutions

Equipment

- Spectrophotometer capable of reading at **240 nm in kinetic mode**

Note

Turn on the equipment at least 15 min before reading or as specified by the manufacturer.

7.4 Solutions

Hydrogen Peroxide (H_2O_2)

- Based on the last concentration check of H_2O_2 (**14.22 M** on June 13, 2024), prepare 10 mL of H_2O_2 solution in water:
 - In a tube (15 mL), add **141 μL** of H_2O_2 from the stock bottle
 - Fill with deionized water up to a total volume of **10 mL**
 - Briefly vortex
 - Wrap the tube in aluminum foil to protect the solution from light
 - Store in the refrigerator at 4°C

Notes

Commercial solutions of H_2O_2 are typically found at concentrations of 30% to 35% (w/w), which corresponds to a molar concentration of approximately 9.8 to 10.3 M. If you are not sure about the concentration of your H_2O_2 stock, prepare dilutions in ratios of 1:50, 1:100, and 1:200 and determine the concentration experimentally as described [below](#).

CAUTION

Use Personal Protective Equipment (PPE). Hydrogen peroxide is a strong oxidizing agent and should be handled with care.

Phosphate Buffer (KPi) + EDTA

The most convenient way to prepare phosphate buffer containing EDTA at the desired pH is to use concentrated solutions of monobasic potassium phosphate (1 M), dibasic potassium phosphate (1 M), and EDTA (500 mM). Mix them in a suitable ratio to achieve the pH close to the desired level and adjust the pH if necessary, as described below.

Monobasic Potassium Phosphate (KH_2PO_4)

- Prepare a 1 M solution of KH_2PO_4 :
 - Molecular Weight: 136.09 g/mol
 - Weigh **13.609 g** of KH_2PO_4
 - Dissolve in approximately 90 mL of deionized water
 - Top up to **100 mL** with deionized water
 - No need to measure or adjust the pH. Store in the refrigerator at 4°C

Dibasic Potassium Phosphate (K_2HPO_4)

- Prepare a 1 M solution of K_2HPO_4 :

- Molecular Weight: 174.18 g/mol
- Weigh **87.09 g** of K_2HPO_4
- Dissolve in approximately 450 mL of deionized water
- Top up to **500 mL** with deionized water
- No need to measure or adjust the pH. Store in the refrigerator at 4°C

Ethylenediaminetetraacetic Acid (EDTA)

- Prepare a 500 mM solution of EDTA:
 - Molecular Weight: 292.24 g/mol
 - Weigh **7.306 g** of EDTA
 - Dissolve in approximately 40 mL of deionized water
 - Adjust the **pH to 8.0** using 1 M NaOH (to increase the pH)
 - After adjusting the pH, top up to **50 mL** with deionized water
 - Store in the refrigerator at 4°C

Note

At this concentration, EDTA will not dissolve completely until the pH is made alkaline.

Phosphate Buffer (KPi) + EDTA

- Using the previous solutions, prepare a 500 mM phosphate buffer containing 5 mM EDTA (pH 7.2):
 - Add **28 mL** of 1 M KH_2PO_4
 - Add **97 mL** of 1 M K_2HPO_4
 - Add 80 mL of deionized water
 - Add **25 mL** of 500 mM EDTA
 - If necessary, adjust the **pH to 7.2** using 1 M HCl (to decrease the pH) or 1 M NaOH (to increase the pH)
 - Top up to **250 mL** with deionized water
 - Aliquot into tubes (50 mL) and store in the refrigerator at 4°C

Note

With the exception of the tube containing the water that will be used in the assay, all solutions (KPi buffer and H_2O_2) and samples should be kept on ice during all procedures.

7.5 Checking H_2O_2 Concentration

In a quartz cuvette:

1. Add **800 μL** of deionized water.
2. Zero the spectrophotometer at **240 nm**.
3. Discard the contents of the cuvette and dry it.
4. Add **40 μL** of the H₂O₂ solution, supposedly at 200 mM.
5. Add **760 μL** of deionized water.
6. Cap the cuvette with a piece of Parafilm and invert it three times to homogenize the contents.
7. Place the cuvette in the holder and record the absorbance at **240 nm**.
8. Discard the contents of the cuvette, wash it, and dry it.
9. Repeat steps 4-8 two more times, obtaining a total of three readings.

Average the three readings and calculate the concentration of H₂O₂ using its molar absorptivity coefficient at 240 nm ($\epsilon_{240} = 0.0394 \text{ mM}^{-1} \text{ cm}^{-1}$):

$$\text{H}_2\text{O}_2 \text{ (mM)} = \left(\frac{(\text{Abs}_1 + \text{Abs}_2 + \text{Abs}_3) / 3}{\epsilon} \right) \times \text{Dilution}$$

Note

Since the dilution used to produce the H₂O₂ solution whose concentration was experimentally determined is known, using the formula $C_1 \cdot V_1 = C_2 \cdot V_2$, it is possible to calculate the concentration in the stock bottle and, from this value, prepare a new solution. This is especially useful when the initially measured concentration is much lower than expected.

Example

Calculating the Concentration

- Reading 1: 0.412 ; Reading 2: 0.402 ; Reading 3: 0.398

$$\begin{aligned} \text{H}_2\text{O}_2 \text{ (mM)} &= \left(\frac{(0.412 + 0.402 + 0.398) / 3}{0.0394} \right) \times 20 \\ \text{H}_2\text{O}_2 \text{ (mM)} &= 205.08 \end{aligned}$$

Note

The dilution factor is 20, as 40 μL of the solution was added to a final volume of 800 μL (40 in 800 = 1:20).

Adjusting the Concentration

The solution described in the example above is slightly more concentrated than 200 mM. Using the formula $C_1 \cdot V_1 = C_2 \cdot V_2$, one can quickly prepare another solution at the correct concentration:

$$205.08 \text{ mM} \times V_1 = 200 \text{ mM} \times 5000 \text{ }\mu\text{L}$$

$$V_1 = \left(\frac{200 \times 5000}{205.08} \right)$$

$$V_1 = 4876.2 \text{ }\mu\text{L}$$

Therefore, to produce a solution of H_2O_2 at 200 mM from a solution whose concentration of 205.08 mM was experimentally verified, it would be necessary to add 4876.2 μL of the solution into a tube and complete to 5000 μL with deionized water.

7.6 Sample Preparation

For this protocol, samples must be homogenized in a way that proteins remain in their native conformations. That is, the homogenate should not have been prepared with high concentrations of detergents or salts, in the presence of chaotropic agents, subjected to heating, or deproteinized. Additionally, the homogenate should be prepared at low temperature and in a buffer containing EDTA and protease inhibitors (see Chapter 5).

7.7 Assay

For this protocol, we will use the **kinetic reading mode**, in which the equipment performs multiple readings at one wavelength over a total period of time. The number of readings during this period depends on the time interval between readings set on the equipment. The interval between readings can be adjusted according to the available equipment, but it is recommended that at least five readings are taken during the total time.

Zero

Before starting kinetic readings, the equipment must be ‘zeroed’ at **240 nm**. To zero the equipment, in a quartz cuvette:

- Add **80 μL** of 500 mM Phosphate Buffer + 5 mM EDTA (pH 7.2)
- Add **720 μL** of Water
- Cap the cuvette with a piece of Parafilm and invert it three times to homogenize the contents
- Place the cuvette in the holder and zero the spectrophotometer at **240 nm**
- Discard the contents of the cuvette and dry it

Note

At a final concentration of 50 mM, the phosphate buffer, which contains 0.5 mM EDTA, shows an approximate absorbance of 0.155 at 240 nm, using a cuvette with a 1 cm optical path. Therefore, it is crucial to calibrate the equipment with the buffer at the final concentration used in the assay, instead of just with water.

Assay Blank

The assay blank is conducted to record changes in absorbance that may occur in the absence of the sample, caused by the components of the reaction medium or their interactions.

For the assay blank, in a quartz cuvette:

- Add **80 μ L** of 500 mM Phosphate Buffer + 5 mM EDTA (pH 7.2)
- Add **680 μ L** of Water
- Add **40 μ L** of 200 mM Hydrogen Peroxide
- Cap the cuvette with a piece of Parafilm and invert it three times to homogenize the contents
- Place the cuvette in the holder and perform the kinetic reading at **240 nm**
- Record the reading
- Discard the contents of the cuvette, wash it, and dry it

Note

For the catalase activity assay, the assay blank should be performed once to diagnose potential issues with the solutions used. Therefore, it is not necessary to repeat the Assay Blank, as long as the initial absorbance is approximately 0.4 and there is no change in absorbance over time.

Sample**Sample Assay**

For the sample assay, in a quartz cuvette:

- Add **80 μ L** of Phosphate Buffer + EDTA (pH 7.2)
- Add **660 μ L** of Water
- Add **20 μ L** of Sample
- Add **40 μ L** of Hydrogen Peroxide
- Cap the cuvette with a piece of Parafilm and invert it three times to homogenize the contents
- Place the cuvette in the holder and perform the kinetic reading at **240 nm**

- Record the reading
- Discard the contents of the cuvette, wash it, and dry it

After the first reading, check the rate of change of absorbance per minute ($\Delta\text{Abs}_{240}/\text{min}$; shown as *rate* or V_{max} depending on the equipment). To avoid abrupt changes in the substrate concentration (H_2O_2) during the reading, **work with rates between -0.025 and -0.035**, which also ensures that the consumption is linear during the reading interval. Therefore, adjust the sample volume to achieve this range, increasing the sample volume if the rate is lower and decreasing it if the rate is higher. Any change in sample volume should be corrected by the water volume to maintain the final volume of 800 μL . For some samples (e.g., rat liver homogenate), it may be necessary to make large dilutions (e.g., 1:2000) and still use a small volume (e.g., 20 μL) to achieve an appropriate rate (between -0.025 and -0.035).

Once the sample volume necessary to achieve a rate of approximately -0.030 has been identified, repeat the reading with this volume two more times, obtaining **a total of three readings** for this sample volume.

Sample Blank

Using the same sample volume identified in the previous section (i.e., the sample volume that causes a $\Delta\text{Abs}_{240}/\text{min}$ of ~ 0.030), record any variations in absorbance at 240 nm caused by the sample itself in the absence of H_2O_2 by performing the reading of the sample blank.

For the sample blank, in a quartz cuvette:

- Add **80 μL** of 500 mM Phosphate Buffer + 5 mM EDTA (pH 7.2)
- Add **700 μL** of Water
- Add **20 μL** of Sample
- Cap the cuvette with a piece of Parafilm and invert the cuvette three times to homogenize the contents
- Place the cuvette in the holder and perform the kinetic reading at **240 nm**
- Record the reading
- Discard the contents of the cuvette, wash it, and dry it
- Repeat two more times, obtaining **a total of three readings** for each sample

Note

For the catalase activity assay, the sample blank typically shows no variation in absorbance at 240 nm over time (i.e., $\Delta\text{Abs}_{240}/\text{min} = 0$). However, this reading also serves to quantify the contribution of the sample itself to the absorbance at 240 nm (i.e., Abs_{240} at the start of the reading). With this value, it is possible to calculate the exact concentration of H_2O_2 at the start of the sample assay reading.

7.8 Expected Results

In this protocol for measuring the activity of catalase, the rates of $\text{Abs}_{240}/\text{min}$ for the Sample Blank and Assay Blank readings are generally equal to 0. That is, there is no consumption of hydrogen peroxide in the absence of the sample and no change in absorbance when the sample is present, but hydrogen peroxide is not (Figure 7.1). On the other hand, in the complete reaction medium, Sample Assay, a decrease in absorbance over time is observed, which corresponds to the consumption of hydrogen peroxide by the catalase present in the sample (Figure 7.1).




Figure 7.1. Representative Readings. Readings illustrating the variation profile of absorbance over the reading time for Assay Blank, Sample Assay, and Sample Blank. For both “blanks,” there is no change in absorbance at 240 nm over time. In the Assay Blank, the absorbance remains at ~ 0.4 (equivalent to 10 mM H_2O_2). In the Sample Blank, the absorbance is near zero due to the absence of H_2O_2 . In the Sample Assay, the absorbance starts near ~ 0.4 (equivalent to 10 mM H_2O_2) and falls linearly during the reading time.

Using increasing amounts of the sample, it is possible to observe an increase in the rate of hydrogen peroxide consumption, corresponding with the increased amount of catalase in the reaction medium (Figure 7.2). However, beyond a certain sample quantity, the amount of catalase becomes excessive, which is evidenced by the non-linearity of the absorbance decrease at 240 nm during the reading. This can be seen in the readings obtained with sample volumes of 10 and 20 μL in the example below (Figure 7.2).

Therefore, one should avoid homogenate volumes that result in very high consumption rates, using a sample amount that falls within the linear range of the relationship between rate (Abs/min) and sample quantity. Under the experimental conditions described in this protocol, the rate (Abs/min) *versus* sample quantity relationship is linear up to approximately $-0.070 \text{ Abs}/\text{min}$ (Figure 7.3). Nevertheless, it is recommended to use a sample volume that results in a rate between -0.025 and -0.035 for all samples. That is, the volume of each sample should be experimentally determined and adjusted, on a case-by-case basis, to achieve Abs/min values within this range.




Figure 7.2. Sample Assay Readings. Absorbance decline profiles at 240 nm using different volumes (0.5 - 20 μL) of rat liver homogenate (1:150, w/v). When there is an excess of sample (e.g., 10 μL), the substrate consumption is so rapid that it causes significant variation in substrate concentration during the reading. This variation affects the enzyme activity during the reading, resulting in a non-linear consumption rate. Note that the initial absorbance differs between the different sample volumes used, as there is consumption of hydrogen peroxide between the time of reagent addition and the start of the reading.

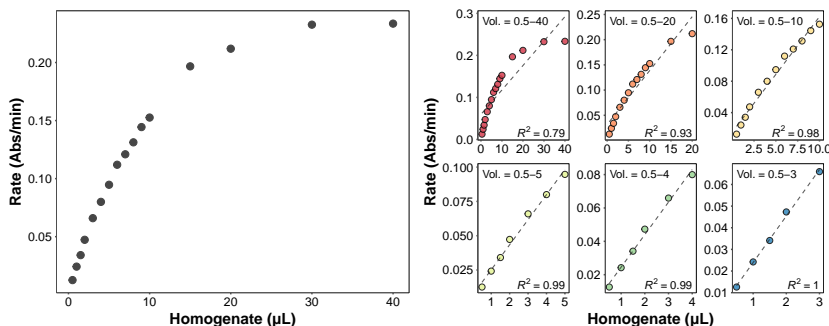


Figure 7.3. H_2O_2 Consumption Rate versus Sample Quantity. Different volumes of rat liver homogenate (1:150, w/v) from 0.5 μL to 40 μL were added in the assay to determine catalase activity. The relationship between Abs/min and sample quantity is linear up to a point where the consumption of H_2O_2 no longer proportionally corresponds to the amount of sample.

7.9 Calculations

Enzymatic activity is often expressed in units per volume (U/mL) or mass (U/mg). An enzyme activity unit (U) is defined as the amount of enzyme that catalyzes the consumption of one micromole of substrate per minute (1 U = $\mu\text{mol}/\text{min}$). In enzymatic assays where the formation of a reaction product is monitored, the unit is defined as the amount of enzyme that catalyzes the production of one micromole of product per minute.

To calculate the activity of catalase in U, we use the formula:

$$\text{Activity (U/mL)} = \left(\frac{\Delta\text{Abs}_{240}/\text{min}}{\varepsilon} \right) \times \text{Dilution 1} \times \text{Dilution 2} \times \text{Dilution 3}$$

where $\Delta\text{Abs}_{240}/\text{min}$ is the change in absorbance at 240 nm per minute (i.e., the rate); ε is the molar absorptivity coefficient; Dilution 1 is the dilution factor performed in the assay; Dilution 2 is the dilution factor performed in the sample preparation; and Dilution 3 is the dilution factor of any other dilution performed.

Note that we are using units per milliliter (U/mL), as, considering that absorbance values are unitless ($\text{Absorbance} = \log_{10} \left(\frac{I_0}{I} \right)$) and the readings were performed in a cuvette with an optical path of 1 cm, dividing $\Delta\text{Abs}_{240}/\text{min}$ by ε results in U/mL:

$$\frac{\text{cm}^{-1}\text{min}^{-1}}{\text{mM}^{-1}\text{cm}^{-1}} = \text{mM} \cdot \text{min}^{-1}$$

Converting:

$$\text{mM} \cdot \text{min}^{-1} = \text{mmol/L} \cdot \text{min}^{-1} = \mu\text{mol/mL} \cdot \text{min}^{-1} = \text{U/mL}$$

Note

Catalase does not follow the usual pattern of Michaelis-Menten kinetics. It is not possible to saturate the enzyme with substrate within a feasible concentration range, and catalase is inactivated by its own substrate at concentrations of H_2O_2 above 100 mM (Aebi 1984). Therefore, some authors recommend not using the International Unit to express catalase activity, but rather the rate constant of a first-order reaction (k).

Example Calculation

The steps to calculate the enzymatic activity of catalase in U include calculating the average $\text{Abs}_{240}/\text{min}$ from technical replicates of the sample assay, correcting the average $\text{Abs}_{240}/\text{min}$ by the average value from technical replicates of the sample blank, calculating the activity in the reaction medium,

adjusting for the dilution performed in the assay, and the final adjustment for the initial dilution of the tissue in the preparation of the homogenate.

Mean Abs₂₄₀/min and Correction by Blank

First, calculate the mean of the Abs₂₄₀/min values recorded for the sample blank and the sample assay. Then, subtract the average value of the sample blank from the average value of the sample assay:

$$\Delta\text{Abs}_{240}/\text{min} = \left(\frac{\text{Assay1} + \text{Assay2} + \text{Assay3}}{3} \right) - \left(\frac{\text{Blank1} + \text{Blank2} + \text{Blank3}}{3} \right)$$

Assuming that a sample resulted in rates of -0.0001, 0.0002, -0.0001 for the sample blank, and -0.03, -0.028, -0.032 for the sample assay, we have:

$$\Delta\text{Abs}_{240}/\text{min} = \left(\frac{-0.03 + -0.028 + -0.032}{3} \right) - \left(\frac{-0.0001 + 0.0002 + -0.0001}{3} \right)$$

$$\Delta\text{Abs}_{240}/\text{min} = (-0.03) - (0)$$

$$\Delta\text{Abs}_{240}/\text{min} = -0.03$$

Note

From this point onward, it is advisable to use the absolute value of the change in absorbance $\Delta\text{Abs}/\text{min}$ (i.e., consider the magnitude without regard to its sign). The sign is negative in this protocol because the molecule being monitored is consumed during the assay, causing a decrease in absorbance over time.

Activity in the Reaction Medium

The corrected average value is divided by the molar absorptivity coefficient of H₂O₂ at 240 nm ($\epsilon_{240} = 0.0394 \text{ mM}^{-1} \text{ cm}^{-1}$) to calculate the activity of catalase in the assay's reaction medium (i.e., the amount of enzyme in the cuvette):

$$\text{Activity (U/mL) in cuvette} = \left(\frac{0.03}{0.0394} \right)$$

$$\text{Activity (U/mL) in cuvette} = 0.761$$

Activity in the Homogenate

To determine the activity of catalase in the homogenate, multiply the activity in the reaction medium by the dilution factor used in the assay (i.e., the final volume of the assay divided by the volume of sample added). For example, if 20 μL of homogenate were added to a final volume of 800 μL , we have a dilution factor of 40:

$$\text{Activity (U/mL) in homogenate} = 0.761 \times \left(\frac{800}{20} \right)$$

$$\text{Activity (U/mL) in homogenate} = 0.761 \times 40$$

$$\text{Activity (U/mL) in homogenate} = 30.46$$

Activity in Tissue

To calculate the activity of catalase in the sample, simply multiply the activity value in the homogenate by any dilutions that have been performed up to the point of assay. The preparation of the homogenate always involves an initial dilution at the time of homogenization. Often, after a centrifugation step, the homogenate is diluted again. Therefore, assuming that a homogenate was initially prepared at a ratio of 1:5 (w/v) (e.g., 100 mg of tissue in 500 μL of final volume) and that after homogenization and centrifugation the homogenate was diluted again 1:400 (e.g., 3 μL of supernatant in 1200 μL of final volume), there is a total dilution factor of 2000:

$$\text{Activity (U/mL) in tissue} = 30.46 \times \left(\frac{500}{100} \right) \times \left(\frac{1200}{3} \right)$$

$$\text{Activity (U/mL) in tissue} = 30.46 \times 5 \times 400$$

$$\text{Activity (U/mL) in tissue} = 30.46 \times 2000$$

$$\text{Activity (U/gww) in tissue} = 60913.71$$

Note

Here, catalase activity is expressed in units per gram of wet weight tissue (U/gww). It is assumed that the density of water (1 g/mL) is an acceptable approximation for the density of biological tissues. If this approximation is not suitable for the sample or tissue being analyzed, catalase activity can be normalized by protein concentration at any of the previous steps, whether in the reaction medium activity or in the homogenate.

Normalization by Protein Concentration

Lastly, to standardize the comparison of enzymatic activity across different samples and experiments, enzymatic activity values are commonly normalized by the amount of protein in the sample. This is done by dividing the calculated activity (U/gww) by the protein concentration in the sample (mg prot./gww). Normalization can be done at any previous step if the protein concentration in the reaction medium or homogenate is known. Assuming that the sample has a protein concentration of 99.1 mg/gww, we have:

$$\text{Activity (U/mg prot.) in tissue} = \left(\frac{6.091371 \times 10^4}{99.1} \right)$$

$$\text{Activity (U/mg prot.) in tissue} = 614.67$$

Note: To normalize enzymatic activity, it is necessary to quantify the protein concentration in the sample using another method (e.g., Bradford assay, BCA, Qubit™, etc.). Quantification should be done using the same homogenate used to measure activity. Refer to protocol CA.002 for protein quantification using the Bradford method.

7.10 3-Amino-1,2,4-Triazole

To ensure that the consumption of H₂O₂ observed in the assay is specifically caused by catalase activity, it is recommended to verify the ability of 3-amino-1,2,4-triazole (ATZ) to reduce the rate of H₂O₂ consumption caused by the sample. ATZ is an irreversible inhibitor of catalase and is used at a concentration of 20 mM with an exposure time of 0.5 to 2.0 hours to abolish catalase activity (Margoliash and Novogrodsky, 1958; [Watanabe and Forman, 2003](https...

Catalase Inhibition by ATZ *in vitro*

The following result illustrates the effect of incubating a sample with ATZ in the absence and presence of H₂O₂. Aliquots of rat liver homogenate were diluted in PBS (resulting in a catalase activity of 40.61 U/mL) and incubated at 22°C for 2.5 hours under three conditions: in the absence of any inhibitor (control), in the presence of 20 mM ATZ (ATZ), and in the presence of 20 mM ATZ + 4 mM H₂O₂ (ATZ + H₂O₂) (Figure 7.4). As the catalase present in the sample consumes H₂O₂ over time, the reaction medium of the ATZ + H₂O₂ treatment was supplemented with H₂O₂ at 0.5-hour intervals to maintain a concentration of 4 mM during the incubation. For the control and ATZ groups, the same volumes of PBS were added to ensure the same dilution factor between treatments.

In the control treatment, catalase activity remained stable throughout the period, oscillating between -0.050 and -0.052 Abs/min. In the ATZ treatment, catalase activity gradually declined, but after 2.5 hours, the inhibition was only 41.3% relative to the initial activity. In the sample treated with ATZ




Figure 7.4. Inhibition of catalase activity by 3-amino-1,2,4-triazole (ATZ). Effect of incubating samples of rat liver homogenate with 20 mM ATZ in the absence and presence of 4 mM H₂O₂ over 2.5 hours. The samples were diluted in PBS, resulting in a catalase activity of 40.61 U/mL, and incubated at 22°C under three different conditions: control (no inhibitors), presence of 20 mM ATZ, and presence of 20 mM ATZ + 4 mM H₂O₂. During the incubation, the reaction medium of the ATZ + H₂O₂ treatment was supplemented with H₂O₂ every 0.5 hours to maintain a constant concentration of 4 mM. In the control and ATZ treatments, equivalent volumes of PBS were added to maintain the same dilution factor.

+ H₂O₂, the activity dropped exponentially, being only 1.5% of the control treatment and the initial activity before the start of the treatment (Figure 4). Therefore, for this sample, all consumption of H₂O₂ can be attributed to catalase activity.

7.11 Additional Comments

Catalase

- Hydrogen Peroxide Concentration:** A concentration of 10 mM H₂O₂ is used to prevent enzyme inactivation during the assay and to minimize the formation of bubbles (O₂) inside the cuvette. Since the concentration of H₂O₂ is critical and at 10 mM the enzyme is not saturated (Figure 7.5), it is essential to always check the stock solution concentration before each assay (see [Hydrogen Peroxide \(H₂O₂\)](#)) and ensure that sample readings start with absorbance values close to 0.4.
- Temperature:** Temperature has a minimal effect on catalase activity (Q_{10} 1.1). Therefore, measurements can be performed over a wide range of temperatures (e.g., 10°C to 37°C) without significant variation ([Aebi 1984](#)). Nonetheless, it is recommended to conduct assays at a consistent temperature (e.g., 25°C or another physiologically relevant temperature for the sample) for samples that will be compared with each other.




Figure 7.5. Rate of H_2O_2 Consumption versus Substrate Concentration. Effect of the final concentration of H_2O_2 on the assay for determining catalase activity. The left panel shows representative readings from assays with final concentrations of 1, 2.5, 5, 10, and 25 mM of H_2O_2 , in addition to the control in the absence of H_2O_2 . Note that at the concentration of 25 mM, the absorbance approaches 1 in a cuvette with a 1 cm optical path. The reading time was reduced to 30 seconds to allow comparison between concentrations, as at 25 mM of H_2O_2 , the Abs/min rate ceases to be linear after 30 seconds under the conditions of the experiment. The right-hand chart shows a linear relationship between substrate concentration and enzymatic activity, indicating that the enzyme is not saturated within this concentration range. The chart displays data from three different readings for each concentration of H_2O_2 .

- **Optimal pH:** Catalase has optimal activity in a pH range of 6.8-7.5 (Aebi 1984).
- **Bubble Formation:** The formation of bubbles during the assay reading of a sample (Figure 6) is an indicator that there is an excess of catalase in the assay and that the reading should be repeated with a smaller sample volume. In addition to indicating excessive substrate consumption, bubbles generate noise in absorbance measurements.
- **Minimizing Pre-Reading H_2O_2 Consumption:** A strategy to minimize the consumption of H_2O_2 between the addition of the sample and the actual start of the reading is to use a piece of Parafilm to position a small volume of sample (5 μL). Cover the cuvette with the Parafilm



Figure 7.6. Bubble Formation. Formation of bubbles (O₂) inside the cuvette after a 1-minute reading. The recorded Abs₂₄₀/min value in this reading was -0.150.

without moving the droplet (Figure ??), invert the cuvette to homogenize the contents, place it in the cuvette holder, and start the reading. This way, the interval between the first contact of the sample with the reaction medium and the start of the reading is minimized, ensuring that the reading actually begins with the final assay concentration of 10 mM H_2O_2 .




Figure 7.7. Minimizing Pre-Reading H_2O_2 Consumption. Steps to ensure rapid initiation of the reading after the sample contacts the reaction medium of the assay. This procedure minimizes the consumption of H_2O_2 before the start of the reading, which is crucial in the absence of automatic injection and mixing systems. Add a volume of up to 5 μL of sample on a piece of Parafilm; carefully cover the cuvette containing buffer, water, and H_2O_2 ; invert the cuvette to homogenize the contents; place it in the holder and start the reading.

Enzymatic Assays

- Temperature Control:** Like common chemical reactions, temperature significantly affects the speed of enzymatic reactions. For most enzyme-catalyzed reactions, the rate increases 2-3 times with every 10°C increase (temperature coefficient, $Q_{10} = 2-3$). That is, an increase in temperature within a specific range accelerates the reaction. To ensure the comparability of results from different samples and experimental days, readings should be made at the same temperature, preferably one that is physiologically relevant to the organism of origin (e.g., 37°C for human tissues). Microplate readers and spectrophotometers have temperature control systems for this purpose. Additionally, it is recommended to keep the deionized water used in the protocol at the assay temperature (e.g., using a water bath or dry block heaters). As most of the reaction medium volume is composed of water, ensuring the water is at the correct temperature helps stabilize the temperature of the reaction medium more quickly.
- pH Control:** Enzymes are sensitive to pH variations and have an optimum pH at which their catalytic activity is maximized. The relationship between enzymatic activity and pH is a bell-shaped curve, with the peak

indicating the optimum pH. From the optimum pH, towards alkaline or acidic extremes, the activity of the enzyme decreases as the pH changes until it finally reaches zero at the extremes. This is because pH affects the ionization of charged groups involved in the catalytic mechanism and/or structural stability of the enzyme. Generally, enzymatic assays are conducted at physiological pH for the organism from which the sample originates. However, in some cases, it is convenient to use a pH that differs from the physiological for analytical reasons.

- **Substrate Concentration:** Ideally, saturating concentrations of substrates and cofactors should always be used to determine an enzyme's activity. However, factors such as high molar absorptivity and low solubility prevent the assay from being conducted at such concentrations in most cases.
- **Initial Rate vs. V_{\max} :** Although some equipment expresses the initial change in absorbance over time (representing the change in substrate or product concentration) in an enzymatic assay as V_{\max} , this value is actually the initial rate (v_0). Note that V_{\max} is a theoretical limit never reached in any experiment, although it is possible to approach it and determine it by extrapolation. This limitation is caused by the fact that complete saturation can only be achieved at infinite concentrations of substrates and cofactors, and, despite using high concentrations of substrates and cofactors, the concentrations cannot be considered as completely saturating.
- **Enzyme Unit:** The enzyme unit, or international unit of enzymatic activity (U, sometimes IU), is a measure of an enzyme's catalytic activity. This unit is defined as the amount of enzyme that catalyzes the conversion of one μmol of substrate per minute ($1 \text{ U} = \mu\text{mol}/\text{min}$), under conditions specified by the assay method.
- **Expression of Enzymatic Activity:** Measures of enzymatic activity are often expressed as units per milligram of protein (U/mg protein), both in cell lysates or tissue homogenates and in isolated protein preparations. This practice is based on the need to normalize enzymatic activity relative to the amount of protein present in the sample, providing a standardized way to compare enzymatic activity between different samples and experiments.

General Observations

- **Volume Adjustments and Optical Path Length:** The final volume and the volumes of reagents can be adjusted for stock solutions of different concentrations and reading containers of different volumes, such as cuvettes or microplates, provided that the final concentrations are maintained as specified in the protocol. It is crucial to adjust the obtained signal for an optical path length of 1 cm, as the molar coefficient indicated in the protocol is in cm^{-1} . This means that if a reading container with a different optical path length is used, the absorbance value should

be multiplied by the ratio between 1 cm and the new path length, ensuring the correct adjustment of the measured signal. For example, if the optical path is 0.5 cm, the measured absorbance should be multiplied by 2.

- **Useful Formulas:** The following formulas are useful for verifying protocol information or adjusting the quantity/volume of the solution, as needed on a case-by-case basis. For all of them, it is important to pay attention to the units of each variable.
 - To prepare dilutions from stock solutions: $C_1 \cdot V_1 = C_2 \cdot V_2$
 - To prepare a new solution from volume and concentration or mass and concentration: $\text{Mass (g)} = \text{Concentration (M)} \cdot \text{Volume (L)} \cdot \text{Molecular Weight (g/mol)}$
 - Lambert-Beer Law: $A = \varepsilon \cdot C \cdot l$, where A is absorbance; ε is the molar absorption coefficient ($\text{M}^{-1} \text{cm}^{-1}$); C is the concentration of the solution (M); l is the path length of the optical path (cm).

7.12 References

Aebi H. 1984. Catalase in vitro. *Methods in Enzymology* 105 121–126. [https://doi.org/10.1016/S0076-6879\(84\)05016-3](https://doi.org/10.1016/S0076-6879(84)05016-3)

Bagnyukova, T.V., Vasyukiv, O.Yu., Storey, K.B., Lushchak, V.I., 2005. Catalase inhibition by amino triazole induces oxidative stress in goldfish brain. *Brain Research* 1052, 180–186. <https://doi.org/10.1016/j.brainres.2005.06.002>

Ho, Y.-S., Xiong, Y., Ma, W., Spector, A., Ho, D.S., 2004. Mice Lacking Catalase Develop Normally but Show Differential Sensitivity to Oxidant Tissue Injury. *Journal of Biological Chemistry* 279, 32804–32812. <https://doi.org/10.1074/jbc.M404800200>

Margoliash, E., Novogrodsky, A., 1958. A study of the inhibition of catalase by 3-amino-1:2:4-triazole. *Biochemical Journal* 68, 468–475. <https://doi.org/10.1042/bj0680468>

Robinson, P.K., 2015. Enzymes: principles and biotechnological applications. *Essays in Biochemistry* 59, 1–41. <https://doi.org/10.1042/bse0590001>

Spitz, D.R., Adams, D.T., Sherman, C.M., Roberts, R.J., 1992. Mechanisms of cellular resistance to hydrogen peroxide, hyperoxia, and 4-hydroxy-2-nonenal toxicity: The significance of increased catalase activity in H_2O_2 -resistant fibroblasts. *Archives of Biochemistry and Biophysics* 292, 221–227. [https://doi.org/10.1016/0003-9861\(92\)90071-4](https://doi.org/10.1016/0003-9861(92)90071-4)

Watanabe, N., Forman, H.J., 2003. Autoxidation of extracellular hydroquinones is a causative event for the cytotoxicity of menadione and DMNQ in A549-S cells. *Archives of Biochemistry and Biophysics* 411, 145–157. [https://doi.org/10.1016/S0003-9861\(02\)00716-6](https://doi.org/10.1016/S0003-9861(02)00716-6)

Weydert, C.J., Cullen, J.J., 2010. Measurement of superoxide dismutase, catalase and glutathione peroxidase in cultured cells and tissue. *Nature Protocols* 5, 51–66. <https://doi.org/10.1038/nprot.2009.197>

Superoxide Dismutase

Bibliography

- Aebi, H. (Jan. 1, 1984). “Catalase in vitro.” In: *Methods in Enzymology* 105, pp. 121–126. DOI: [10.1016/S0076-6879\(84\)05016-3](https://doi.org/10.1016/S0076-6879(84)05016-3). URL: <http://www.sciencedirect.com/science/article/pii/S0076687984050163> (visited on 10/12/2019) (cit. on p. 20).
- Bagnyukova, T. V., O. Y. Vasyukiv, K. B. Storey, and V. I. Lushchak (Aug. 9, 2005). “Catalase inhibition by amino triazole induces oxidative stress in goldfish brain.” In: *Brain Research* 1052.2. Number: 2, pp. 180–186. DOI: [10.1016/j.brainres.2005.06.002](https://doi.org/10.1016/j.brainres.2005.06.002). URL: <https://www.sciencedirect.com/science/article/pii/S0006899305008498> (visited on 07/06/2022) (cit. on p. 20).
- Ho, Y.-S., Y. Xiong, W. Ma, A. Spector, and D. S. Ho (July 2004). “Mice Lacking Catalase Develop Normally but Show Differential Sensitivity to Oxidant Tissue Injury.” In: *Journal of Biological Chemistry* 279.31, pp. 32804–32812. DOI: [10.1074/jbc.M404800200](https://doi.org/10.1074/jbc.M404800200). URL: <https://linkinghub.elsevier.com/retrieve/pii/S0021925820775812> (visited on 06/27/2024) (cit. on p. 20).
- Spitz, D. R., D. T. Adams, C. Sherman, and R. J. Roberts (Jan. 1992). “Mechanisms of cellular resistance to hydrogen peroxide, hyperoxia, and 4-hydroxy-2-nonenal toxicity: The significance of increased catalase activity in H₂O₂-resistant fibroblasts.” In: *Archives of Biochemistry and Biophysics* 292.1, pp. 221–227. DOI: [10.1016/0003-9861\(92\)90071-4](https://doi.org/10.1016/0003-9861(92)90071-4). URL: <https://linkinghub.elsevier.com/retrieve/pii/0003986192900714> (visited on 06/27/2024) (cit. on p. 20).

Abstract English abstract, on the last page. English abstract, on the last page.English abstract, on the last page.English abstract, on the last page.English abstract, on the last page.English abstract, on the last page.English abstract, on the last page.English abstract, on the last page.

Keywords Keyword1, Keyword2, Keyword3, Keyword4, Keyword5.

