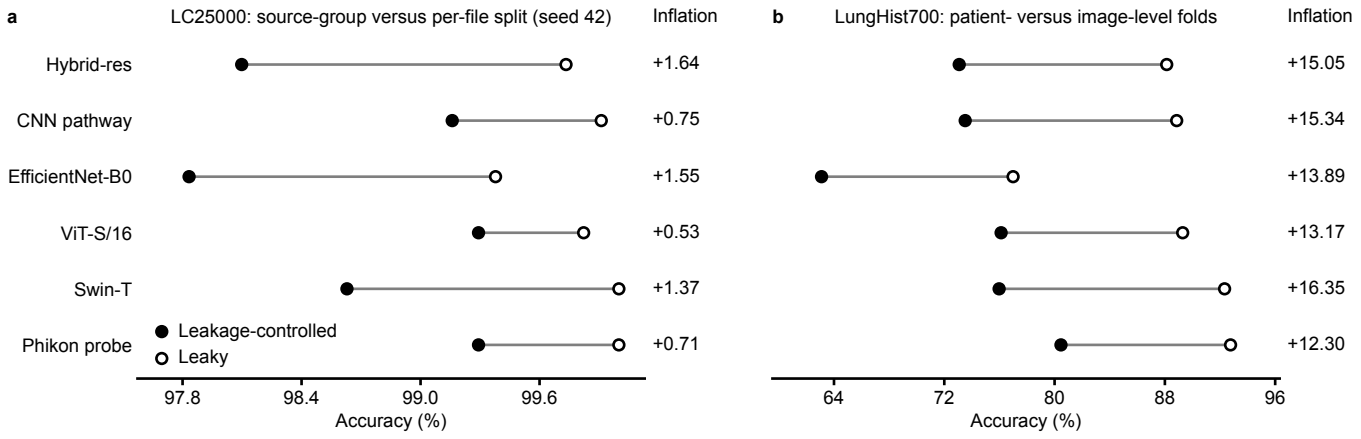
a
LC25000: source-group versus per-file split (seed 42)
Inflation
Hybrid-res
CNN pathway
EfficientNet-B0
ViT-S/16
Swin-T
Phikon probe
+1.64
+0.75
+1.55
+0.53
+1.37
+0.71
Leakage-controlled
Leaky
97.8
98.4
99.0
99.6
Accuracy (%)
b
LungHist700: patient- versus image-level folds
Inflation
+15.05
+15.34
+13.89
+13.17
+16.35
+12.30
64
72
80
88
96
Accuracy (%)