

Translation and Rotation Properties of DI ($n = 20$)

Observed sample after transformation
Original sample position
Original-to-transformed movement
Optimal medoid-sample match
IPnM medoid (reference unit)


(a) Original sample
Starting configuration
DI = 0.00; MI = -0.47; VI = 0.01; BI = 0.04

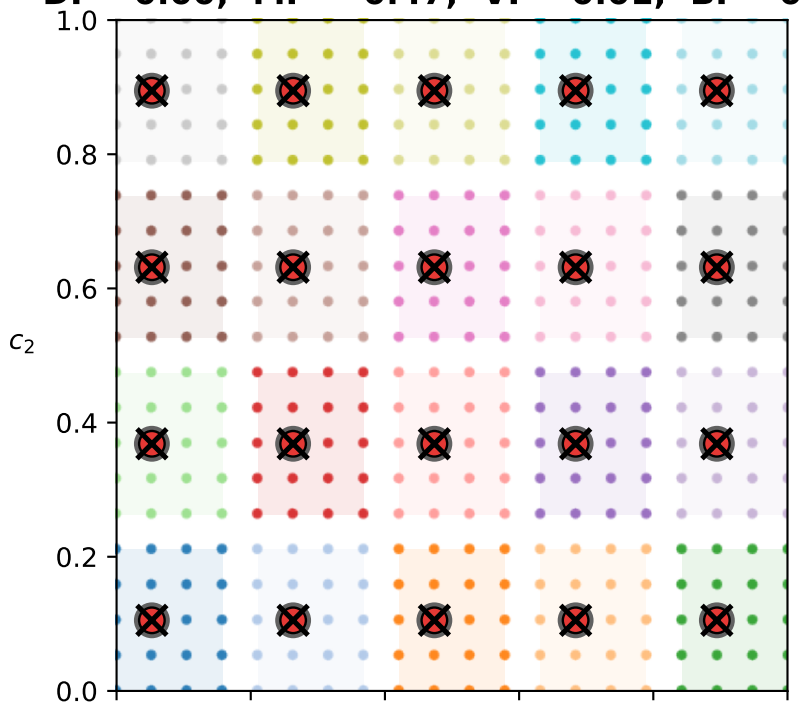

(b) Uniformly shifted sample
Same shift applied to every sample point
DI = 0.00; MI = -0.44; VI = 0.03; BI = 0.08

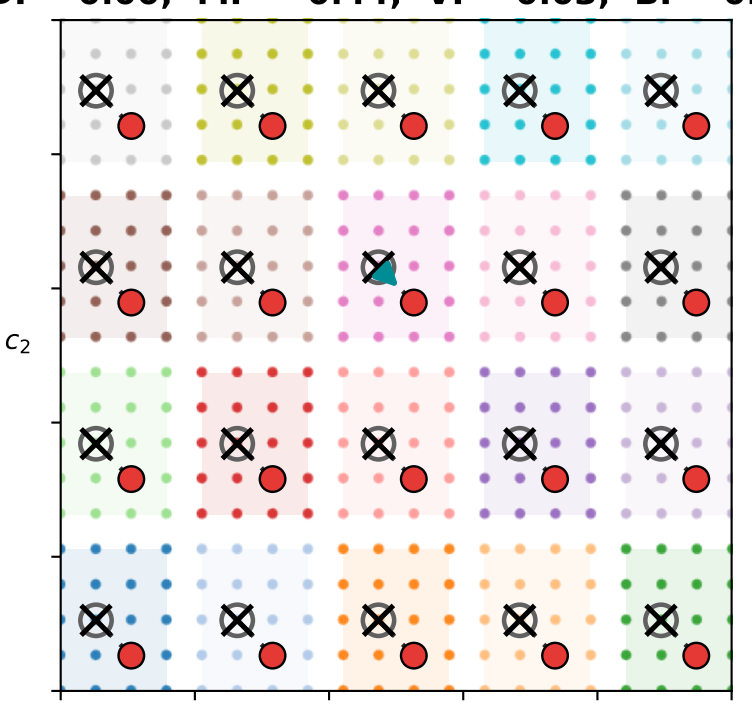

(c) Sample rotated 90 ° **Counterclockwise about the sample center**
DI = 0.00; MI = -0.47; VI = 0.01; BI = 0.04

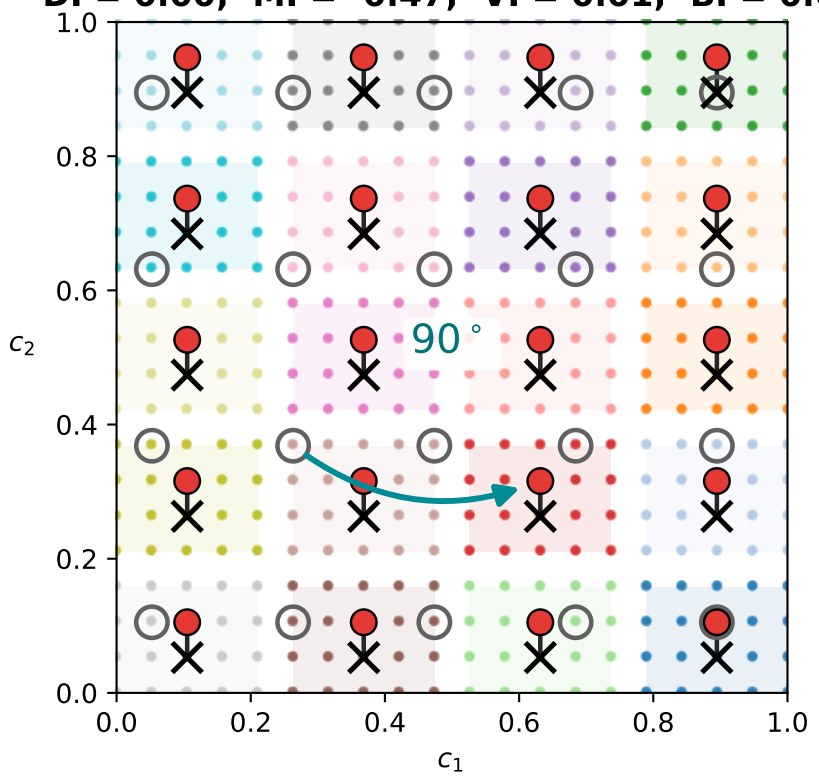

(d) Sample rotated 45 ° **Counterclockwise about the sample center**
DI = -0.14; MI = -0.23; VI = 0.15; BI = 0.19

