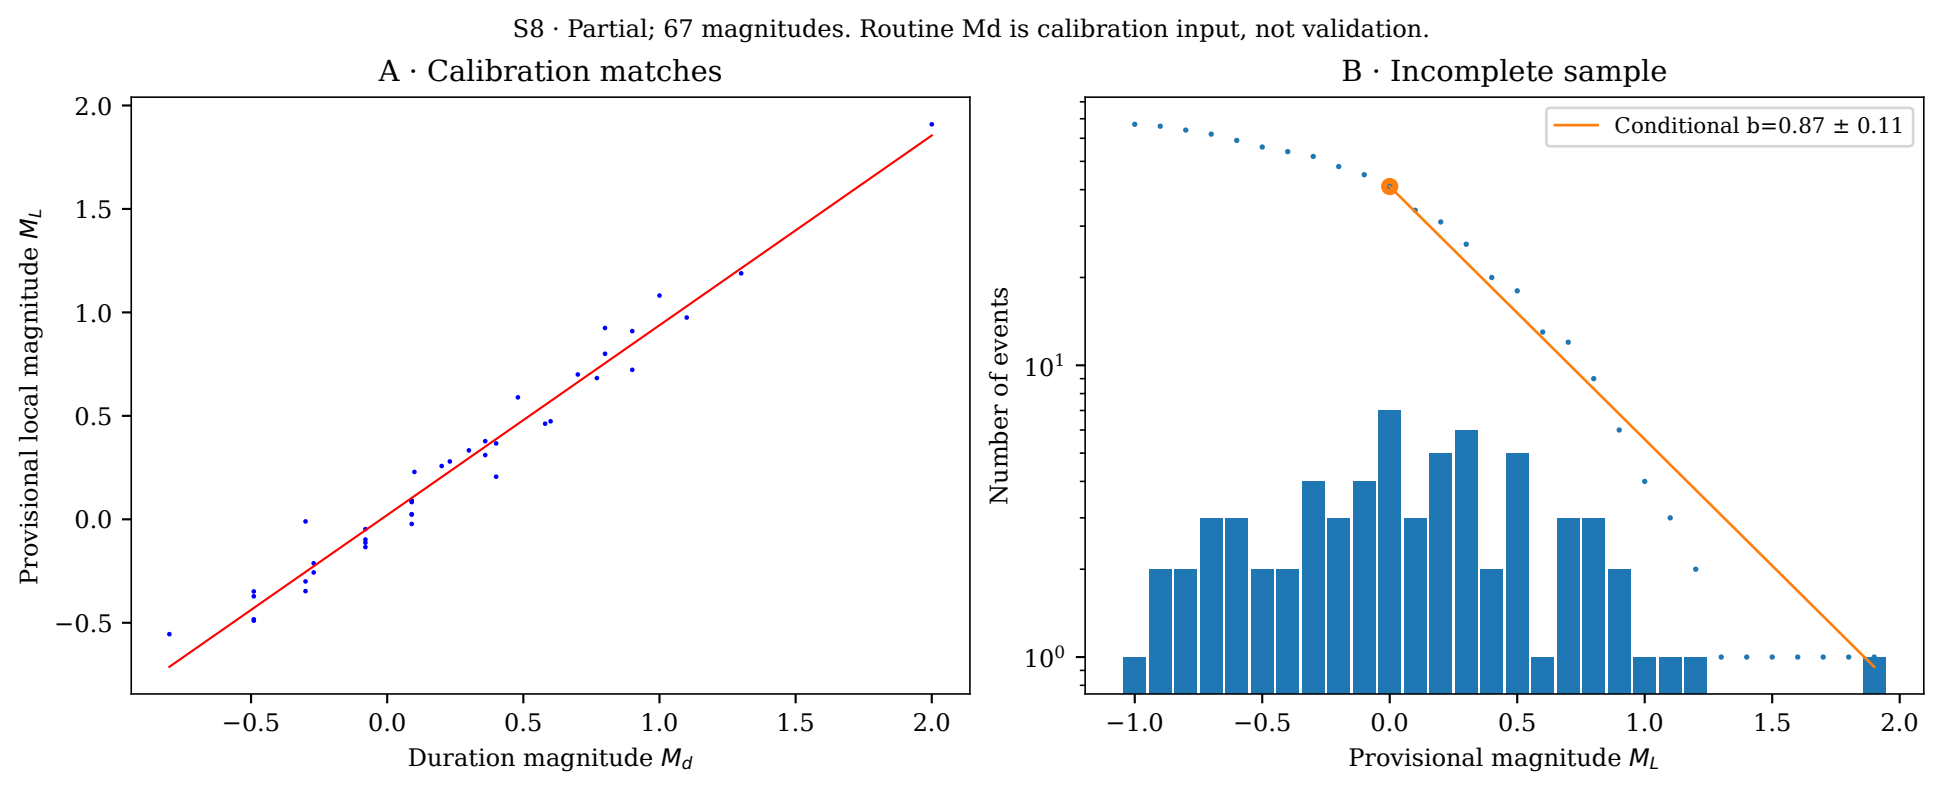
S8 · Partial; 67 magnitudes. Routine Md is calibration input, not validation.
A · Calibration matches
Provisional local magnitude $M_L$
Duration magnitude $M_d$
B · Incomplete sample
Conditional b=0.87 ± 0.11
Number of events
Provisional magnitude $M_L$