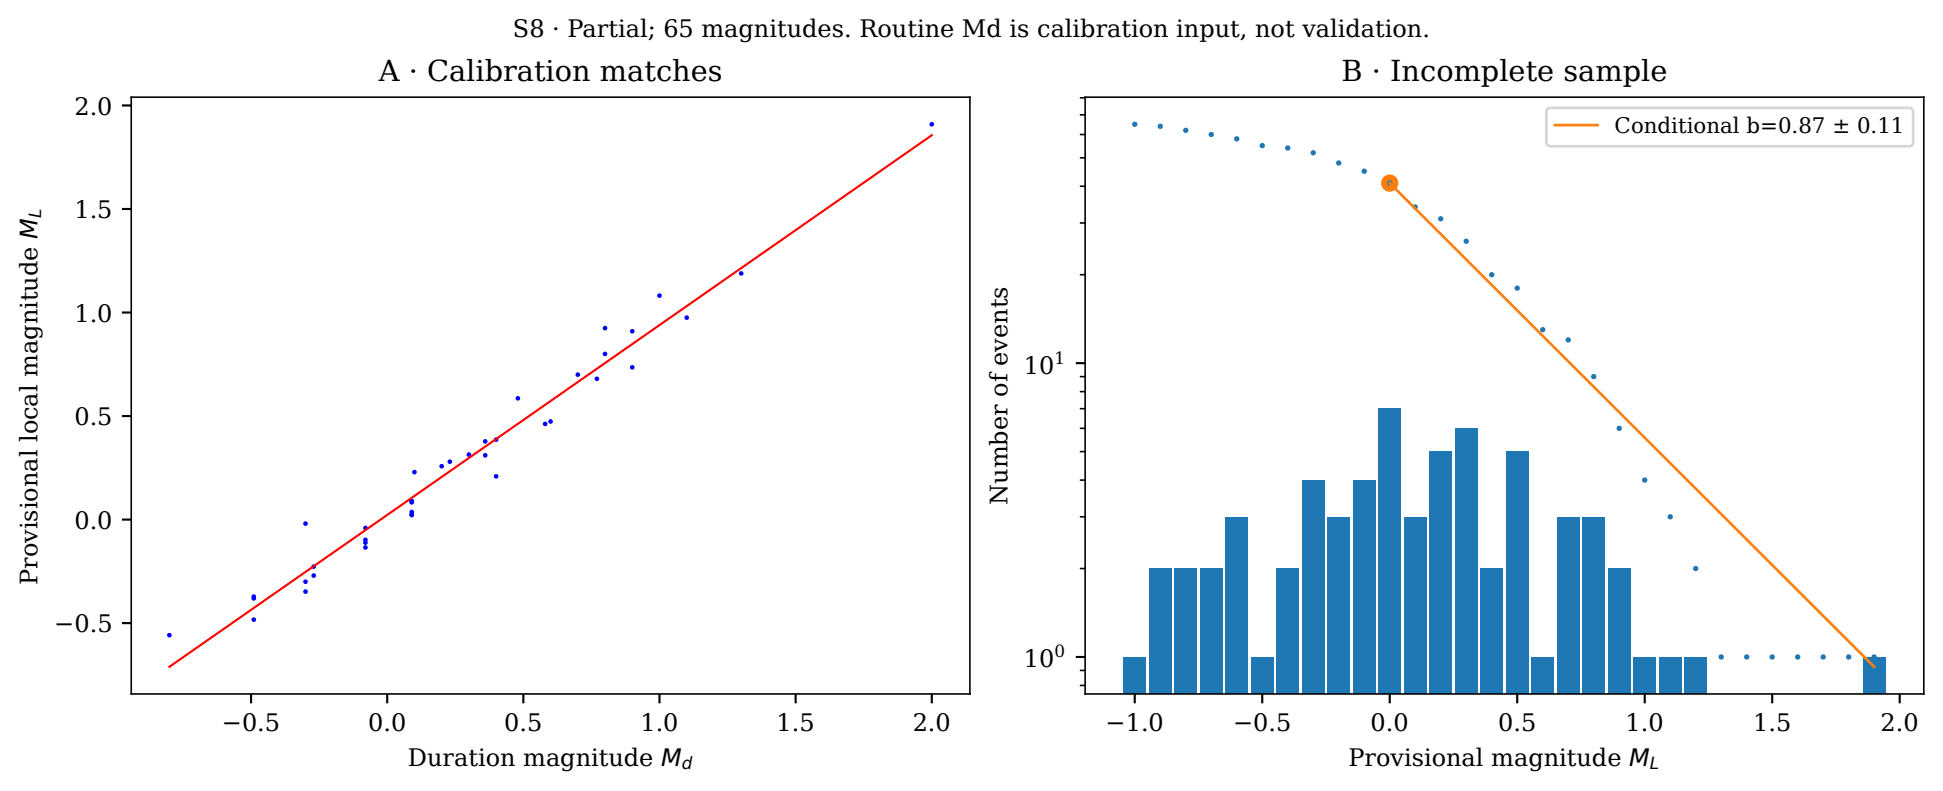
S8 · Partial; 65 magnitudes. Routine Md is calibration input, not validation.
A · Calibration matches
Provisional local magnitude M_L
Duration magnitude M_d
B · Incomplete sample
Conditional b=0.87 ± 0.11
Number of events
Provisional magnitude M_L