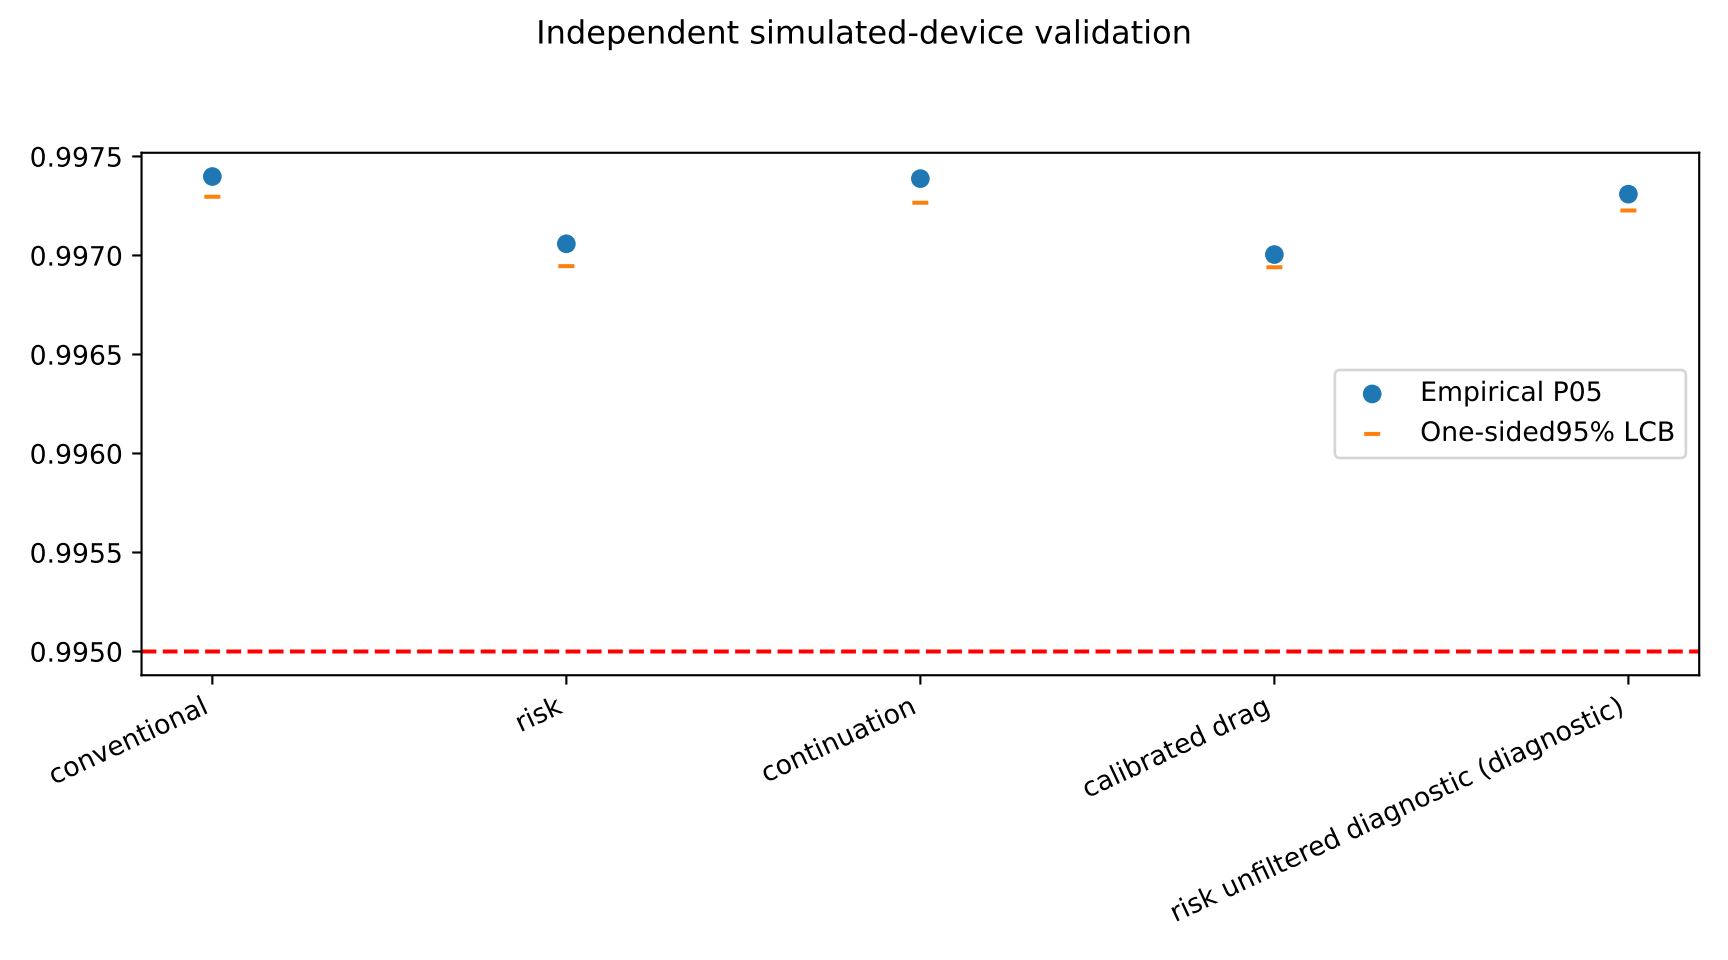
Independent simulated-device validation
0.9975
0.9970
0.9965
0.9960
0.9955
0.9950
Empirical P05
One-sided95% LCB
conventional
risk
continuation
calibrated drag
risk unfiltered diagnostic (diagnostic)