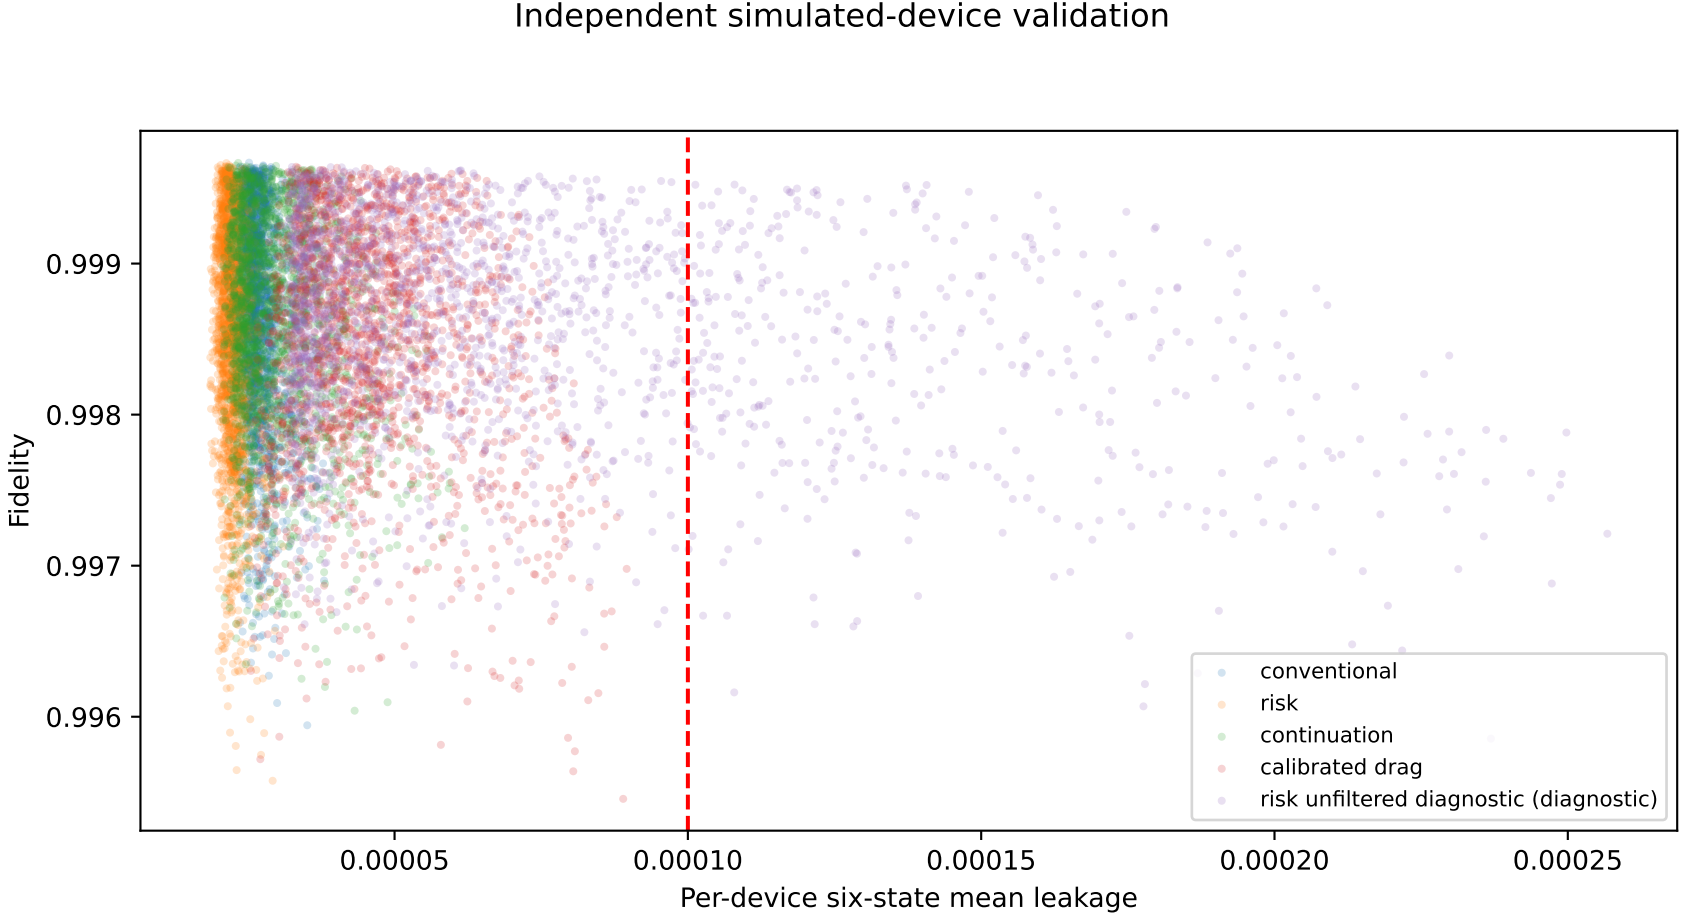

Independent simulated-device validation
Fidelity
0.999
0.998
0.997
0.996
0.00005
0.00010
0.00015
0.00020
0.00025
Per-device six-state mean leakage
conventional
risk
continuation
calibrated drag
risk unfiltered diagnostic (diagnostic)