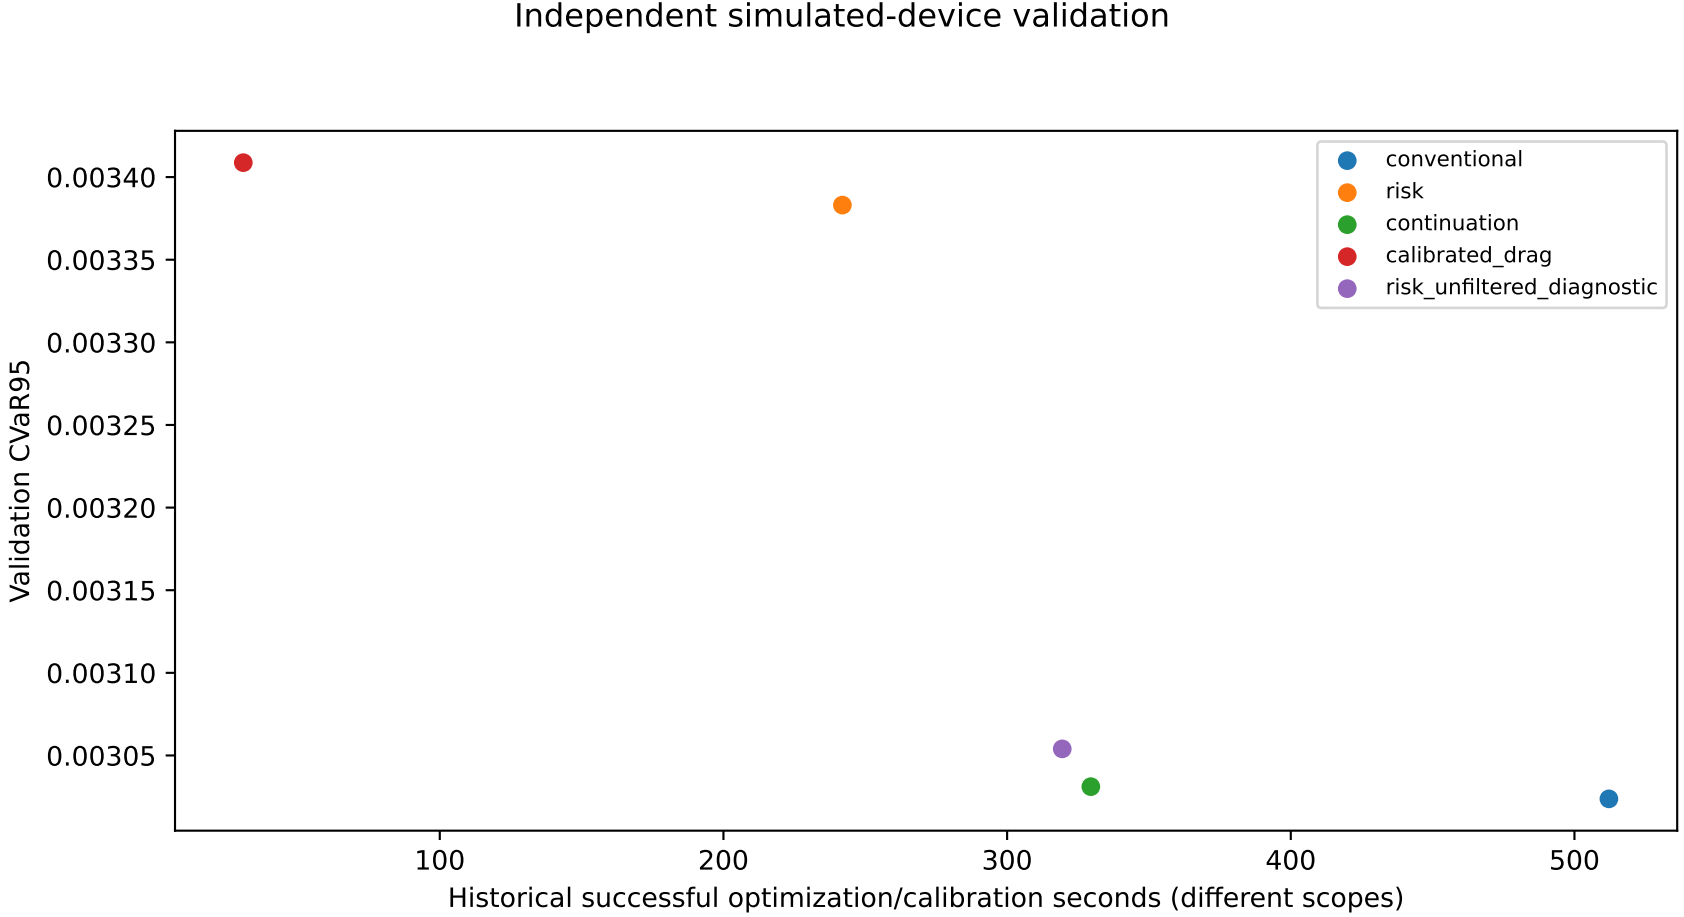
Independent simulated-device validation
Validation CVaR95
0.00340
0.00335
0.00330
0.00325
0.00320
0.00315
0.00310
0.00305
100
200
300
400
500
Historical successful optimization/calibration seconds (different scopes)
conventional
risk
continuation
calibrated_drag
risk_unfiltered_diagnostic