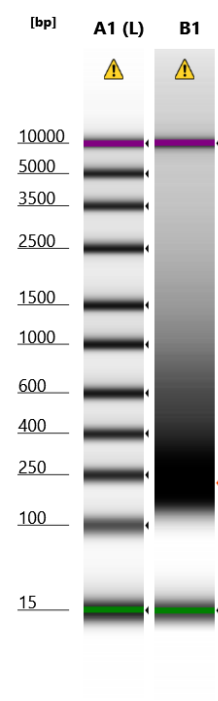


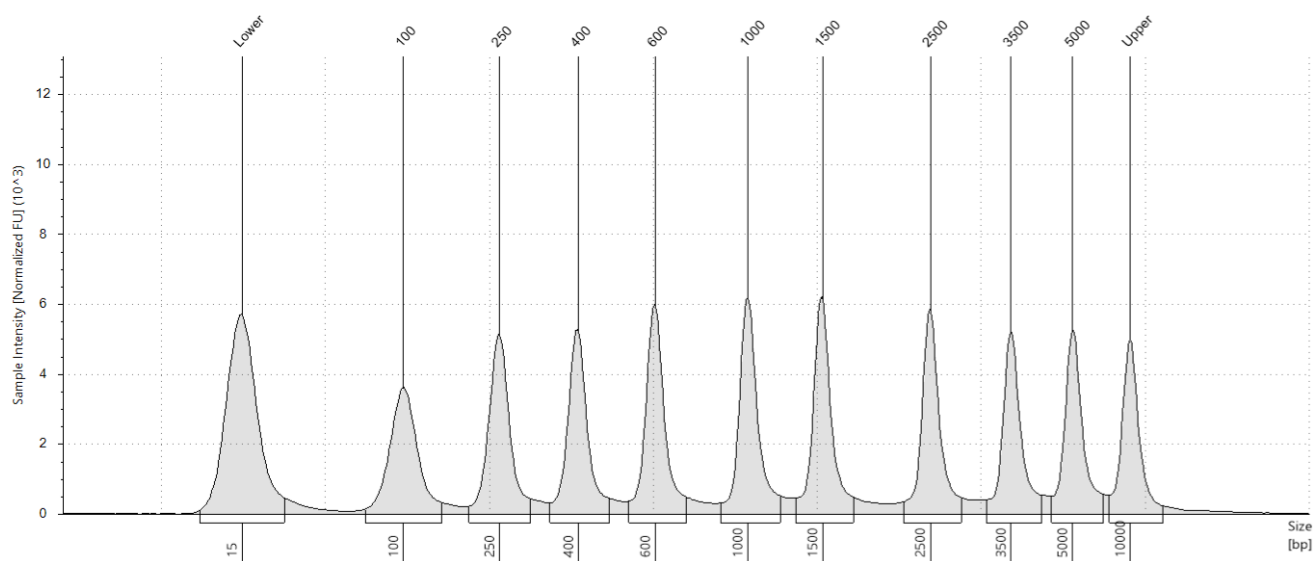
Filename: 2019-08-16 - 14.26.59.D5000



Default image (Contrast 100%)

Sample Info

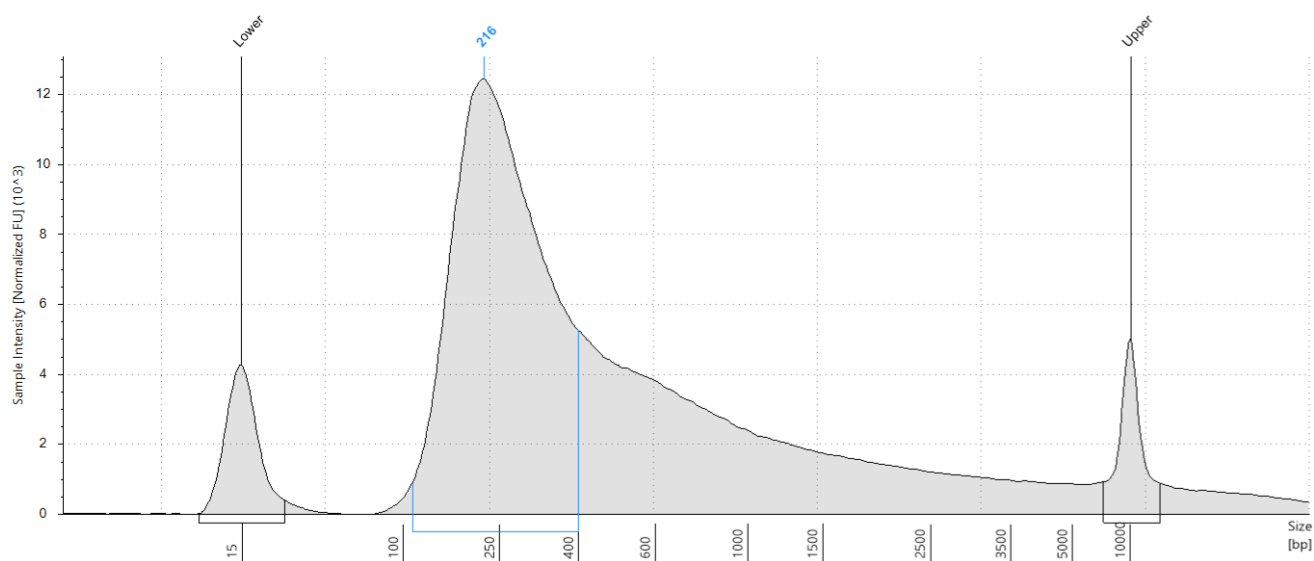
Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	45.5	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1	59.1	Block 12 Biotinylated Probes	⚠	Caution! Expired ScreenTape device

**A1: Ladder****Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	45.5	Ladder	⚠	Caution! Expired ScreenTape device; Ladder

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.54	-	773	-		Lower Marker
100	4.85	-	74.7	10.67		
250	5.17	-	31.8	11.36		
400	4.99	-	19.2	10.97		
600	5.42	-	13.9	11.91		
1000	5.49	-	8.45	12.08		
1500	5.40	-	5.54	11.87		
2500	5.01	-	3.08	11.00		
3500	4.58	-	2.01	10.06		
5000	4.59	-	1.41	10.08		
10000	3.25	3.25	0.500	-		Upper Marker

**B1: Block 12 Biotinylated Probes****Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	59.1	Block 12 Biotinylated Probes	⚠	Caution! Expired ScreenTape device

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.43	-	659	-		Lower Marker
216	59.1	-	420	100.00		
10000	3.25	3.25	0.500	-		Upper Marker