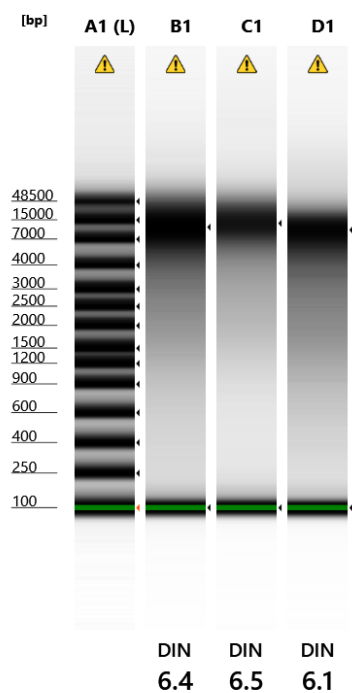


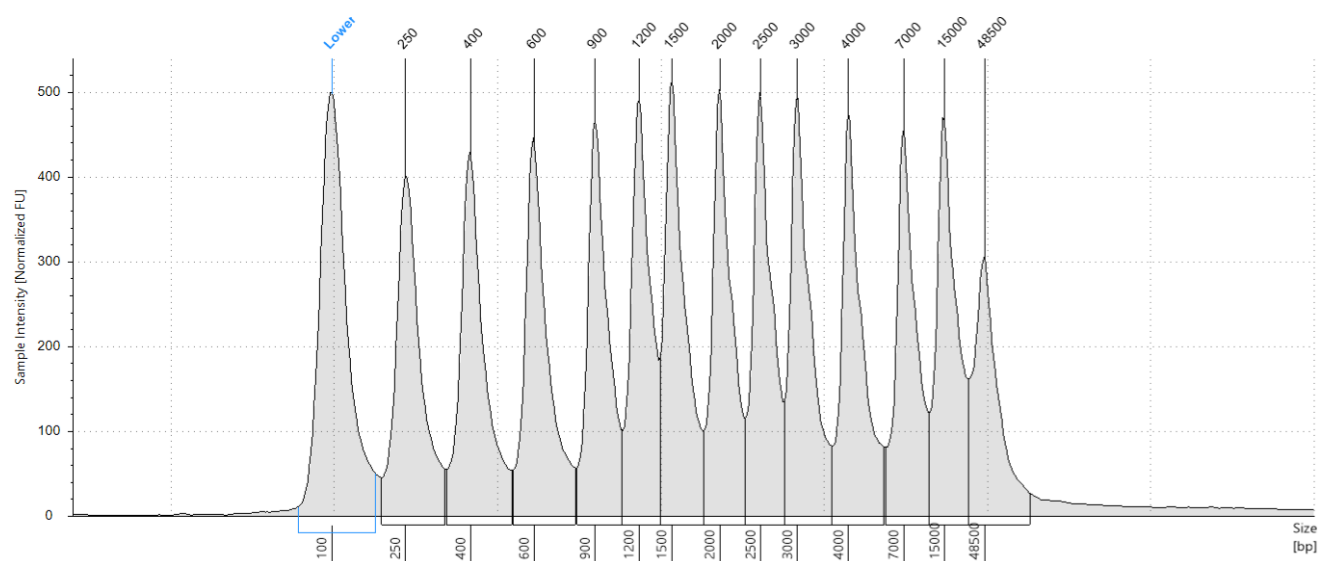
Filename: 2020-08-04 - 12.50.20.GDNA



Default image (Contrast 100%)

### Sample Info

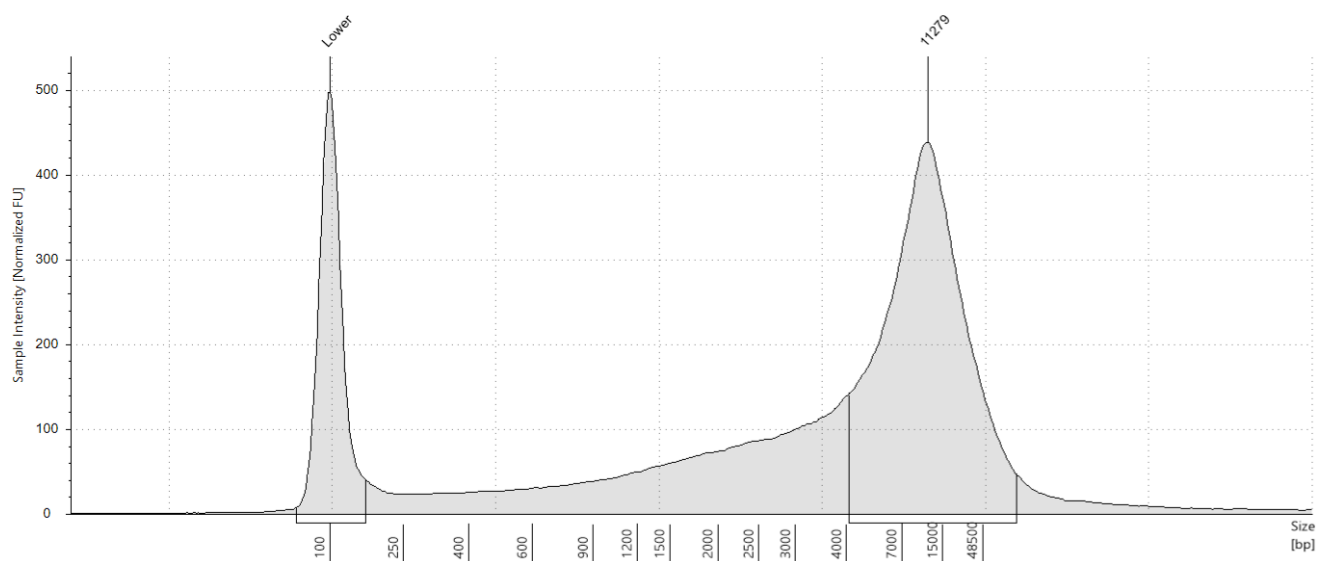
Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	A1	-	77.3	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
	B1	6.4	44.0	797	⚠	Caution! Expired ScreenTape device
	C1	6.5	29.5	822	⚠	Caution! Expired ScreenTape device
	D1	6.1	40.3	887	⚠	Caution! Expired ScreenTape device

**A1: Ladder****Sample Table**

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	77.3	Ladder	⚠	Caution! Expired ScreenTape device; Ladder

**Peak Table**

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	66	173	131	
250	6.05	-	7.87	185	333	37.3	
400	6.26	-	8.13	336	519	24.1	
600	6.22	-	8.09	524	789	15.9	
900	5.80	-	7.55	796	1074	9.92	
1200	6.02	-	7.82	1074	1388	7.71	
1500	6.56	-	8.53	1388	1822	6.73	
2000	5.95	-	7.74	1822	2297	4.58	
2500	5.92	-	7.70	2297	2817	3.64	
3000	6.20	-	8.06	2817	3634	3.18	
4000	5.94	-	7.72	3634	5726	2.28	
7000	5.52	-	7.18	5809	11234	1.21	
15000	5.86	-	7.62	11234	23479	0.601	
48500	4.60	-	5.98	23479	86786	0.146	

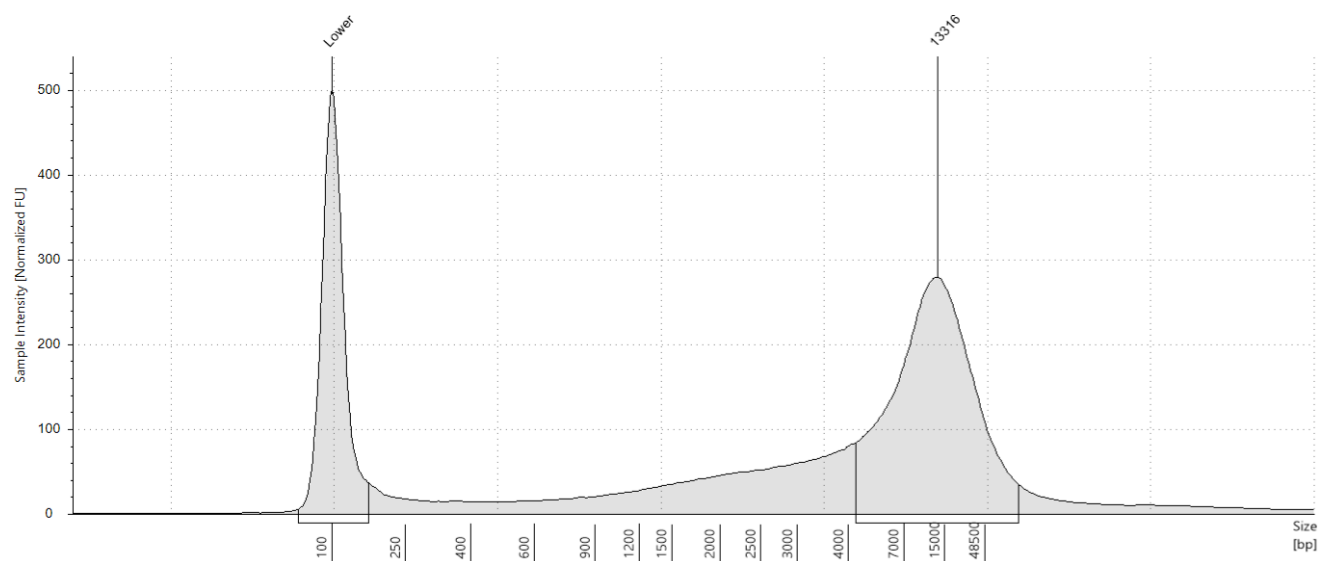
**B1: 797****Sample Table**

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	B1	6.4	44.0	797	⚠	Caution! Expired ScreenTape device

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	66	155	131	
11279	25.7	-	96.37	4081	>60000	3.51	
-	-	-	-	-	-	-	

## C1: 822

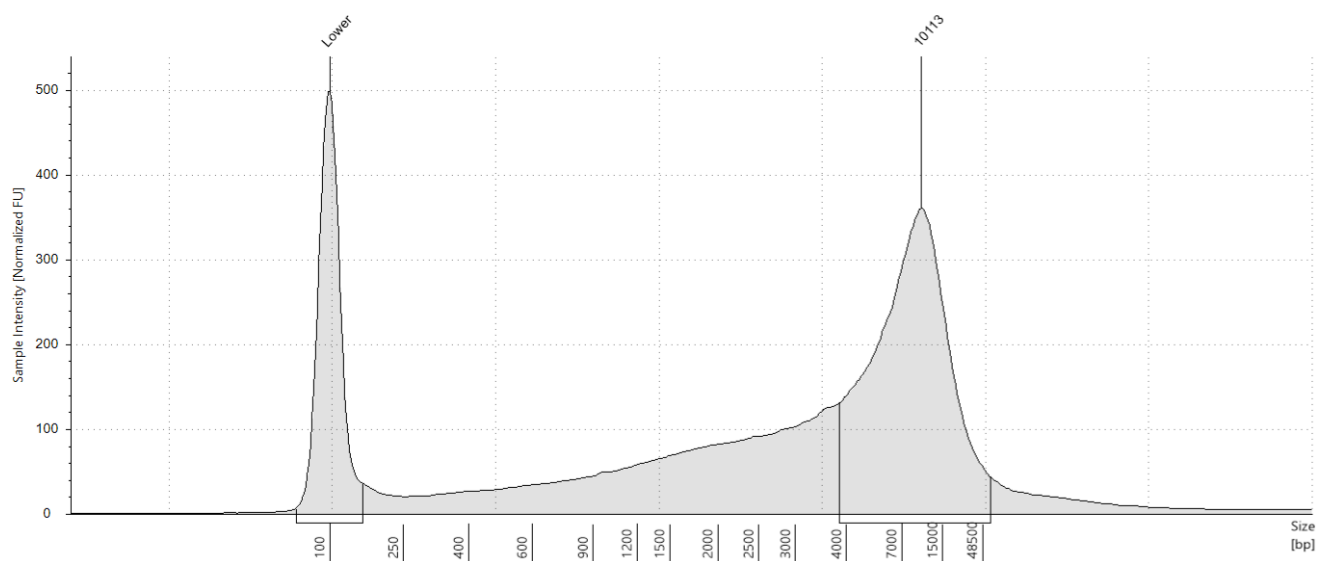


## Sample Table

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	C1	6.5	29.5	822	⚠	Caution! Expired ScreenTape device

## Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	65	158	131	
13316	17.2	-	96.15	4323	>60000	1.98	
-	-	-	-	-	-	-	

**D1: 887****Sample Table**

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	D1	6.1	40.3	887	⚠	Caution! Expired ScreenTape device

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	66	150	131	
10113	20.3	-	95.25	3843	55679	3.09	
>60000	0.236	-	1.11	>60000	>60000	-	
-	-	-	-	-	-	-	