

Bitcrusher

Audio Signal Modification Unit
User Manual And Technical Reference

ACOUSTIC RESEARCH



In this our 20th year of operation, and on behalf of the entire company; I would personally like to express my deepest gratitude for your continued support of our products and services.

Here at Acoustic Research, we pride ourselves in the quality of our instruments and ensure that every one meets the high standards that our customers deserve. I have no doubt, that the equipment that you have received today will meet those standards just as they did 20 years ago.

I wish you the greatest success in your research

James Chaffinch
James Chaffinch, CEO

References in this publication to Acoustic Research products, programs, or services do not imply that Acoustic Research intends to make these available in all countries in which Acoustic Research operates. Any reference to an Acoustic Research product, program or service is not intended to state or imply that only Acoustic Research's product, program, or service may be used. Any functionally equivalent product, program, or service that does not infringe any of Acoustic Research's intellectual property rights or other legally protectable rights may be used instead of the Acoustic Research product, program, or service. Evaluation and verification of operation in conjunction with other products, programs, or services, except those expressly designated by Acoustic Research, are the user's responsibility.

Acoustic Research may have patents or pending patent applications covering subject matter in this document. The furnishing of this document does not give you any license to these patents. You can send license inquiries, in writing, to an Acoustic Research authorized dealer or your Acoustic Research marketing representative, who will be able to forward on the request.

The following terms in this publication are trademarks of Acoustic Research Inc. In the European Union and/or other countries / economic areas.

- Acoustic Research
- Bitcrusher

This publication could include technical inaccuracies or typographical errors. Changes are periodically made to the information herein; these changes will be incorporated in new editions of the publication. Acoustic Research may make improvements and/or changes in the product(s) and/or the program(s) described in this publication at any time.

It is possible that this publication may contain reference to, or information about, Acoustic Research products (machines and programs), programming, or services that are not announced in your country. Such references or information must not be construed to mean that Acoustic Research intends to announce such Acoustic Research products, programming, or services in your country.

Requests for technical information about Acoustic Research products or services for those products, whether they be repair, maintenance or upgrade; should be made to your Acoustic Research authorized dealer or your Acoustic Research marketing representative.

This product's connections follow the Coordinated Universal Interworking Standard (C UIS) and as such can be used with any other product from any manufacturer that also adheres to this standard.

Contents

| | |
|---------------------------------------|---|
| Description | 1 |
| Down-Sampling Of Amplitude Resolution | 1 |
| Down-Sampling Of Sample Frequency | 2 |
| Interface | 3 |
| Unit Specifications | 5 |

Description


The Bitcrusher unit is an audio signal modification device which implements a digital down-sampling algorithm to both the amplitude of a signal, and the temporal opportunities for registered change in that signal known as the sample frequency.

These two down-sampling operations can be analyzed individually, as they do not deeply interact with each other beyond modifying aspects of the signal. In effect, one can perform both operations in any order and produce the same output.

Down-Sampling Of Amplitude Resolution

The amplitude resolution of a signal refers to the number of possible amplitudes that a signal could have. Typically in analogue circuitry this resolution is fine enough to be functionally infinite, but this is not so in digital circuits.

One purpose of the Bitcrusher then, is to quantize the fine resolution signal to a more discrete set of values. The unit achieves this by rounding values to closest available “levels”. Levels are evenly spaced values from -1 to 1. The number of levels is defined as the value of the Amplitude Resolution Dial by 2, plus 1. In essence, an even number of levels either side of zero, plus the zero level itself.

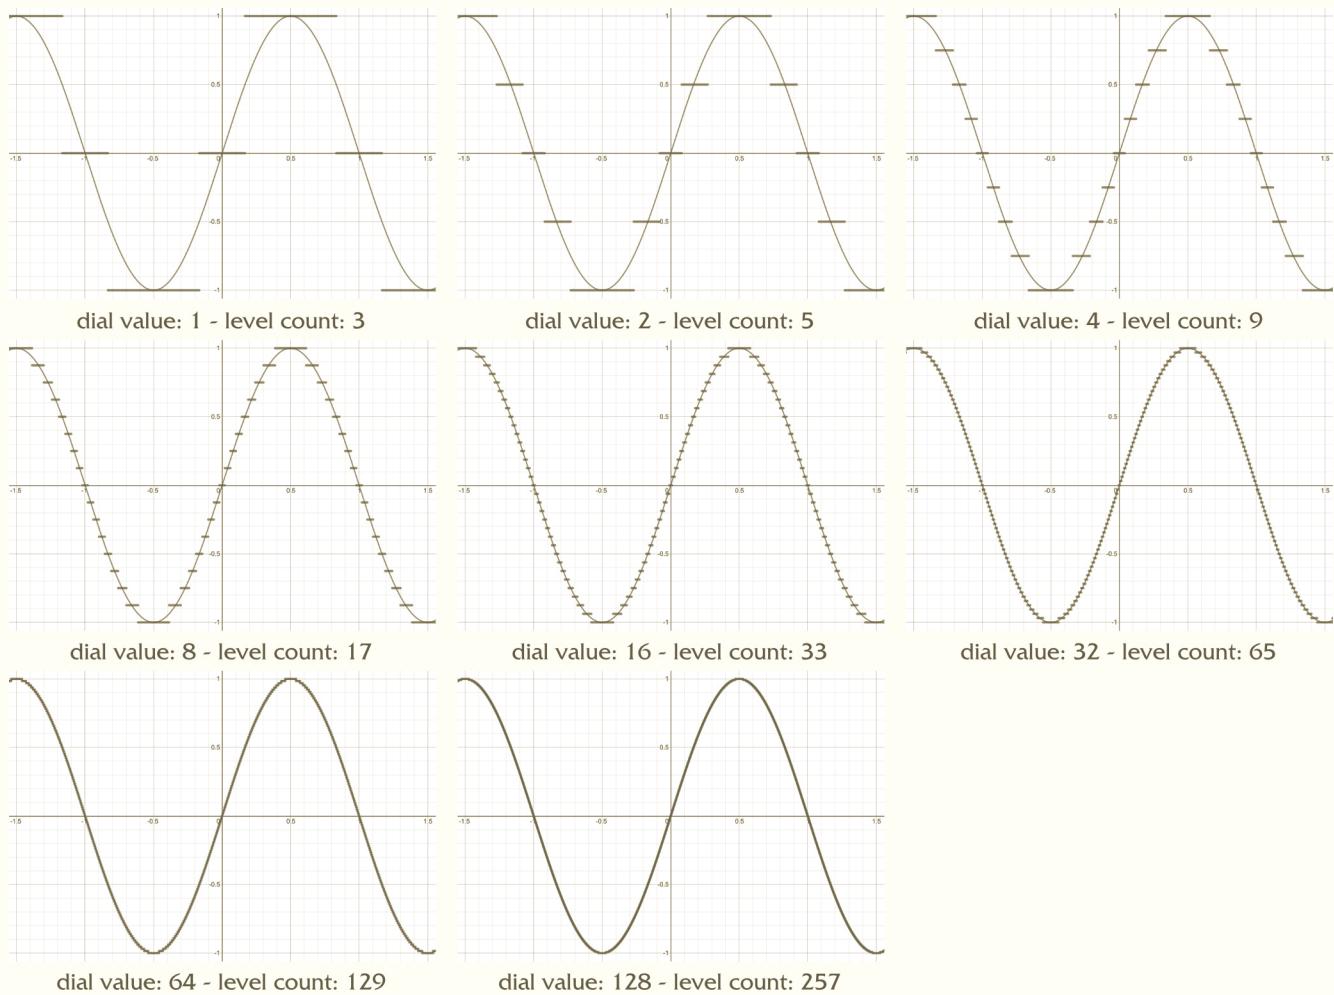


Down-Sampling Of Sample Frequency


The sample frequency of a signal refers to the number times the unit reads the value of the incoming signal over a second. For example, the unit's maximum sampling rate is 128, which means that every 1/128th of a second, it will read what the input signal value is and set the output to this value.

Lowering the number of samples that are taken in a second, results in the output signal losing temporal detail. That is to say, that the resolution in time is reduced, leading to what some have described as a blocky graph.


Think of it like pixilation of an image; less pixels means less detail.

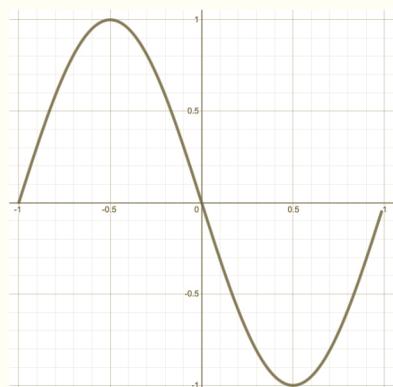


128 samples

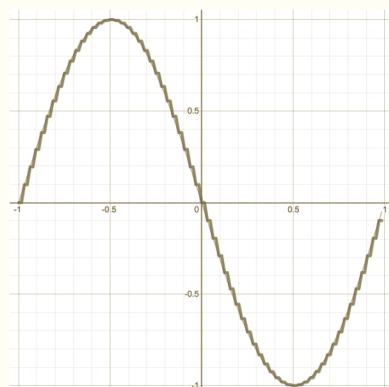


64 samples

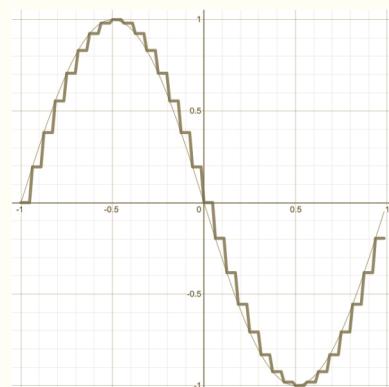


32 samples

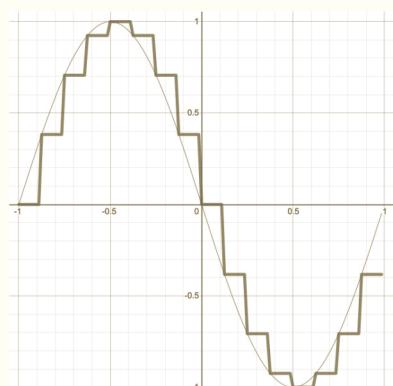


16 samples

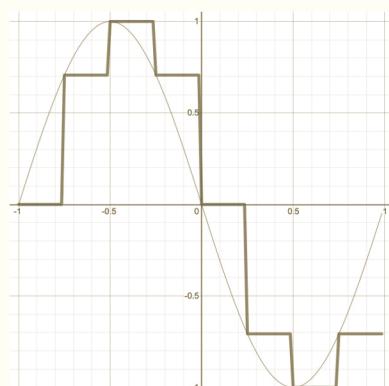


8 samples

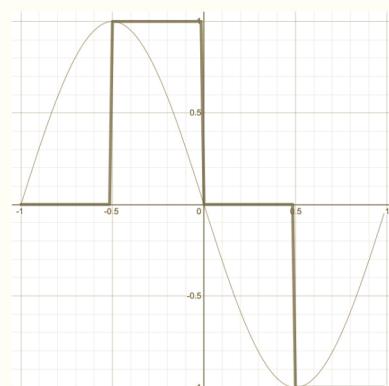

4 samples

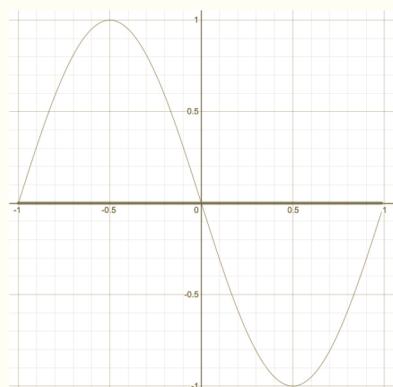

2 samples

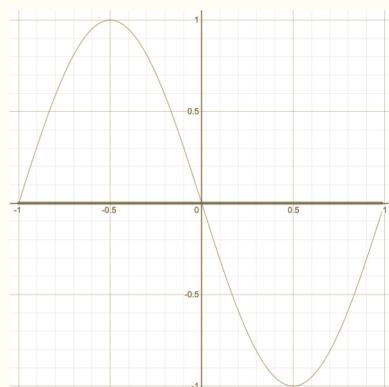


1 sample

Note; the graphs for “2 samples” and “1 sample” are the same, as a result of a trick of math. “1 sample” keeps the value of $x = -1$, which is 0.

“2 samples” keeps the values of $x = -1$ and then $x = 0$, which are both 0.

Interface

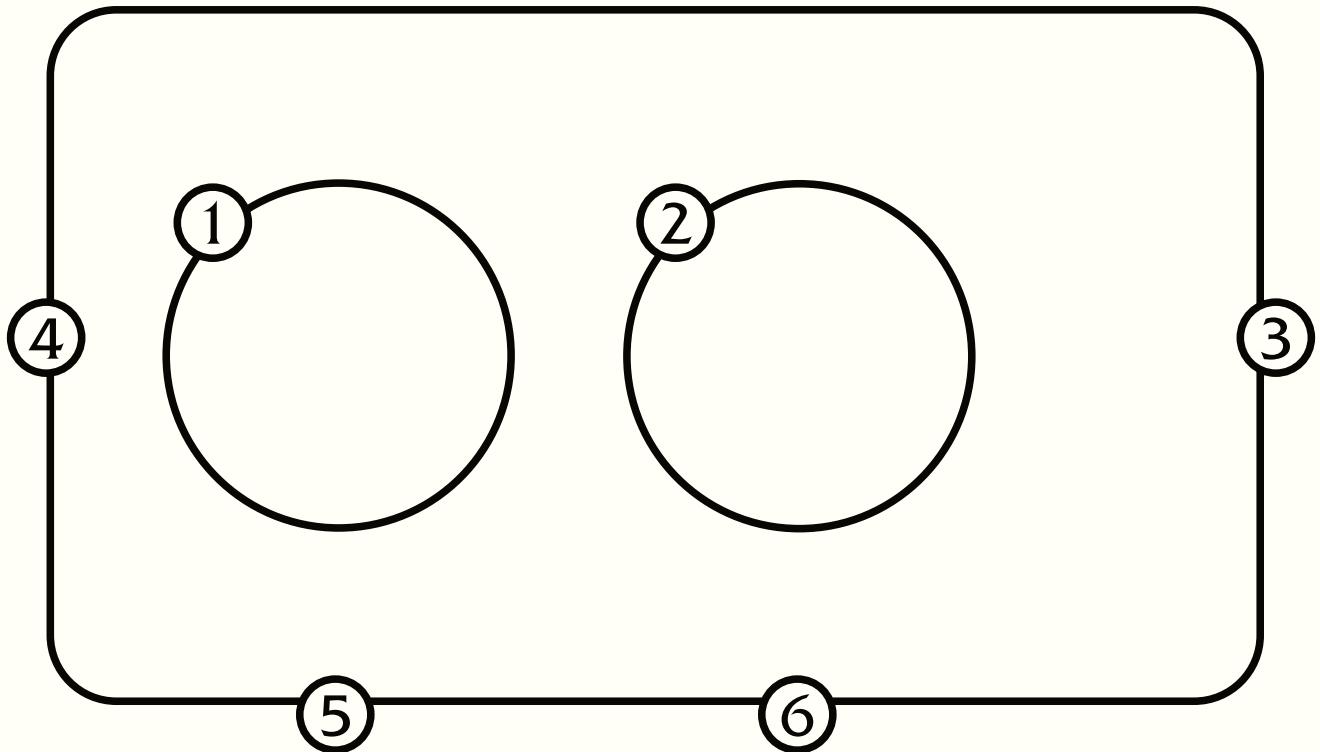

1. Amplitude Resolution Dial

Used to define the value used in the down-sampling of a signal's amplitude.

2. Sample Frequency Dial

Used to select the number of samples the unit will take of the incoming signal over the course of one second.

3. Amplitude Resolution Dial Voltage Control

A voltage control input connection port which directly modifies the Amplitude Resolution Dial (1). Control is between the values of 0 and 1.

CUIS type: Green

4. Sample Frequency Dial Voltage Control

A voltage control input connection port which directly modifies the Sample Frequency Dial (2). Control is between the values of 0 and 1.

CUIS type: Green

5. Audio Signal Input

The audio signal input connection


CUIS type: Orange

6. Audio Signal Output

The audio signal output

CUIS type: Orange

Unit Specifications

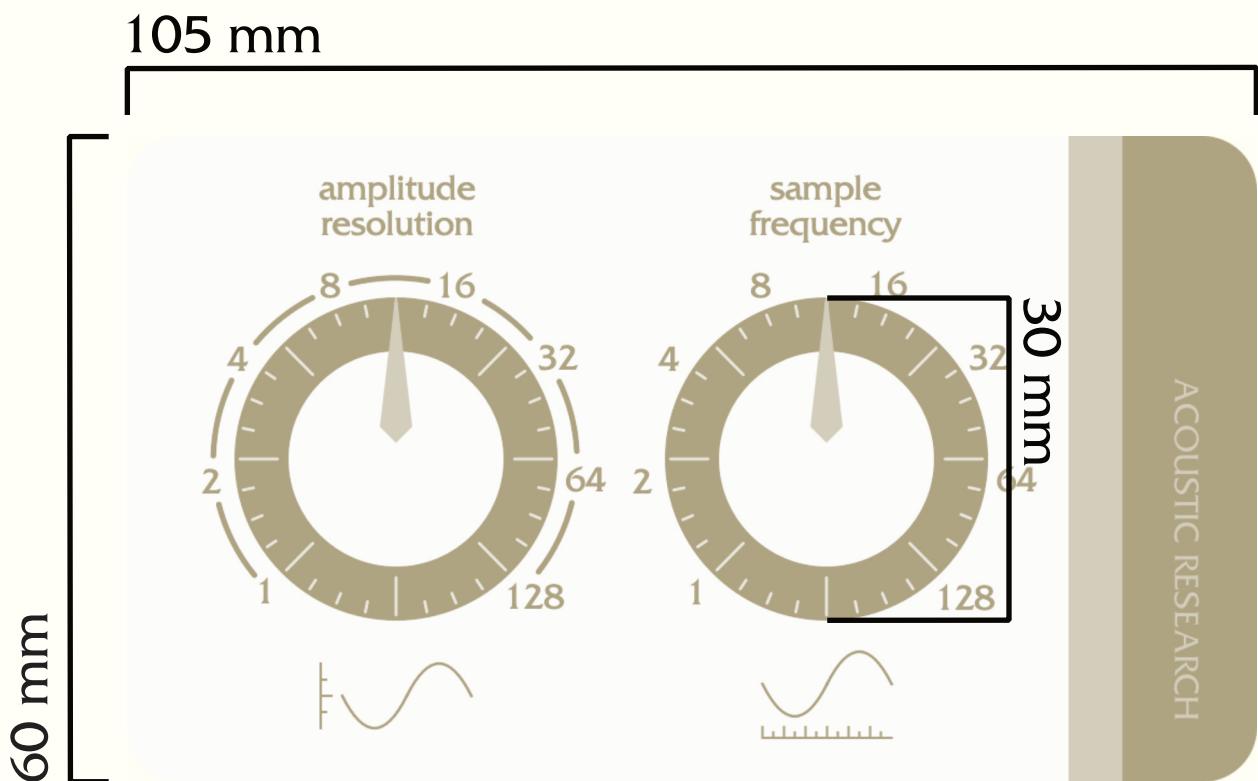

© Copyright Acoustic Research Inc. 1981. All rights reserved