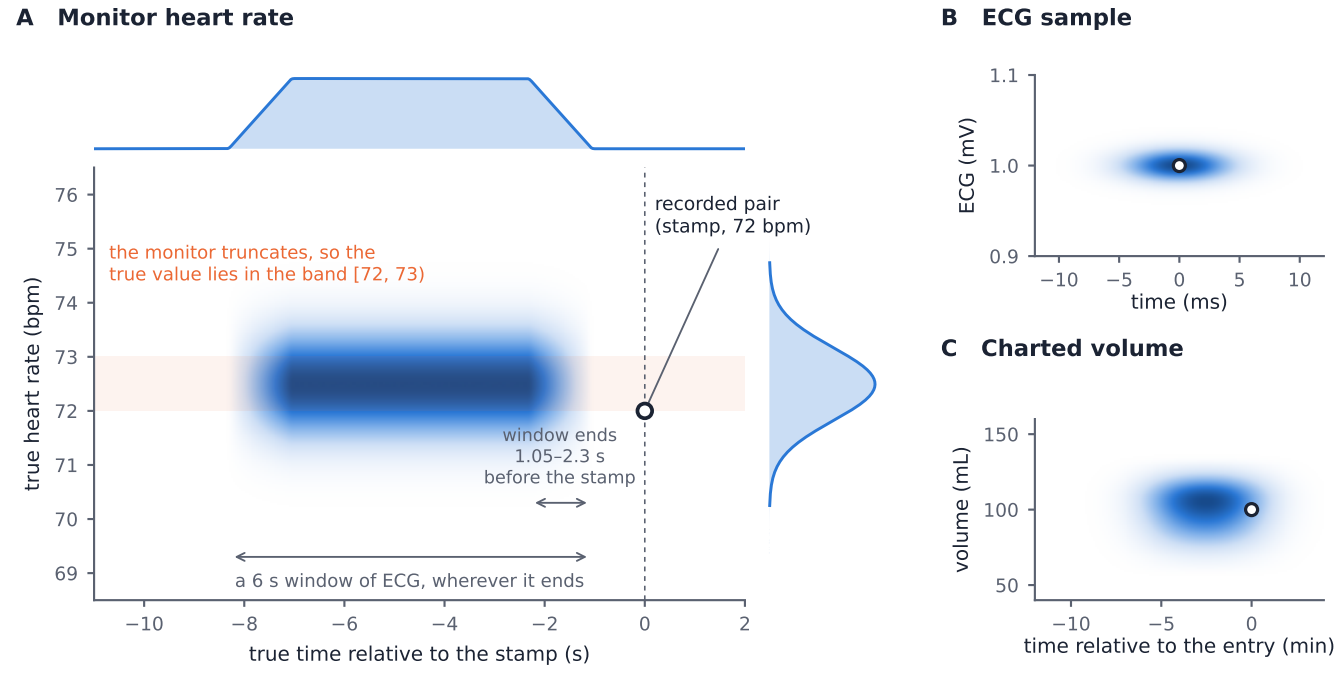

A Monitor heart rate
B ECG sample
C Charted volume
true heart rate (bpm)
true time relative to the stamp (s)
the monitor truncates, so the
true value lies in the band [72, 73)
recorded pair
(stamp, 72 bpm)
window ends
1.05–2.3 s
before the stamp
a 6 s window of ECG, wherever it ends
ECG (mV)
time (ms)
volume (mL)
time relative to the entry (min)