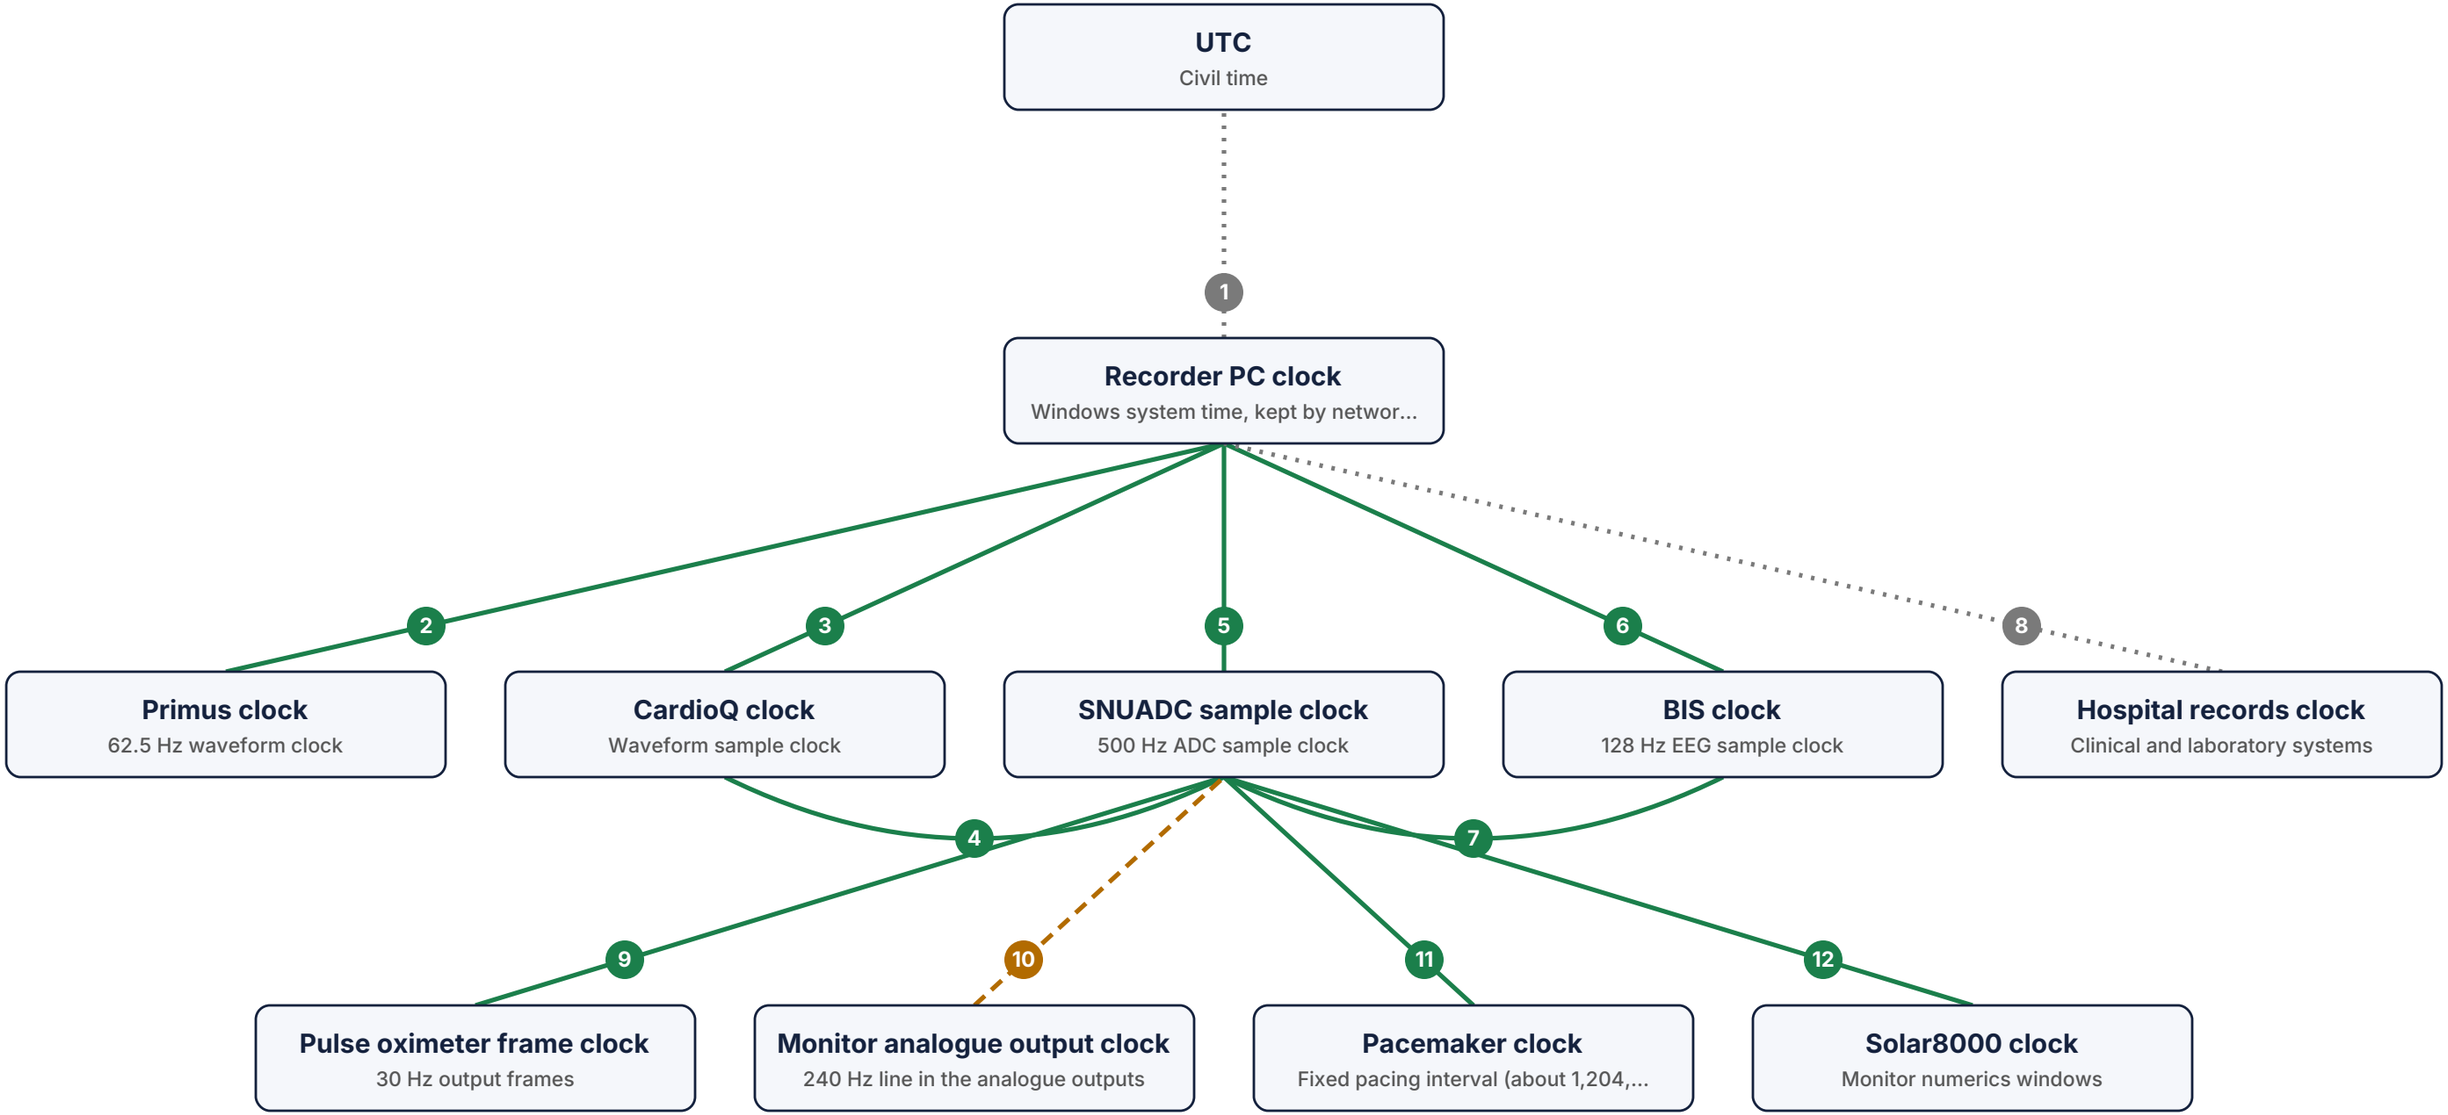
UTC
Civil time
1
Recorder PC clock
Windows system time, kept by networ...
2
3
5
6
8
Primus clock
62.5 Hz waveform clock
CardioQ clock
Waveform sample clock
SNUADC sample clock
500 Hz ADC sample clock
BIS clock
128 Hz EEG sample clock
Hospital records clock
Clinical and laboratory systems
4
7
9
10
11
12
Pulse oximeter frame clock
30 Hz output frames
Monitor analogue output clock
240 Hz line in the analogue outputs
Pacemaker clock
Fixed pacing interval (about 1,204,...
Solar8000 clock
Monitor numerics windows
measured
estimated
assumed
Numbers: the links in the table below. Hover for detail; click to open a page.